



12-1991

Improving neutron dosimetry using bubble detector technology

Mark Alan Buckner

Follow this and additional works at: https://trace.tennessee.edu/utk_gradthes

Recommended Citation

Buckner, Mark Alan, "Improving neutron dosimetry using bubble detector technology. " Master's Thesis, University of Tennessee, 1991.

https://trace.tennessee.edu/utk_gradthes/12355

This Thesis is brought to you for free and open access by the Graduate School at TRACE: Tennessee Research and Creative Exchange. It has been accepted for inclusion in Masters Theses by an authorized administrator of TRACE: Tennessee Research and Creative Exchange. For more information, please contact trace@utk.edu.

To the Graduate Council:

I am submitting herewith a thesis written by Mark Alan Buckner entitled "Improving neutron dosimetry using bubble detector technology." I have examined the final electronic copy of this thesis for form and content and recommend that it be accepted in partial fulfillment of the requirements for the degree of Master of Science, with a major in Nuclear Engineering.

L. F. Miller, Major Professor

We have read this thesis and recommend its acceptance:

Accepted for the Council:

Carolyn R. Hodges

Vice Provost and Dean of the Graduate School

(Original signatures are on file with official student records.)

To the Graduate Council:

I am submitting herewith a thesis written by Mark A. Buckner entitled "Improving Neutron Dosimetry Using Bubble Detector Technology." I have examined the final copy of this thesis for form and content and recommend it be accepted in partial fulfillment of the requirements for the degree of Master of Science, with a major in Nuclear Engineering.

L. F. Miller

L. F. Miller, Major Professor

We have read this thesis
and recommend its acceptance:

Pete J. Jovi
C. S. Juma

Accepted for the Council:

C. W. Mink

Associate Vice Chancellor
and Dean of The Graduate School

STATEMENT OF PERMISSION TO USE

In presenting this thesis in partial fulfillment of the requirements for a Master's degree at the University of Tennessee, Knoxville, I agree that the Library shall make it available to borrowers under the rules of the Library. Brief quotations from this thesis are allowable without special permission, provided that accurate acknowledgement of the source is made.

Permission for extensive quotation from or reproduction of this thesis may be granted by my major professor, or in his absence, by the Head of Interlibrary Services when, in the opinion of either, the proposed use of the material is for scholarly purposes. Any copying or use of the material in this thesis if for financial gain shall not be allowed without my written permission.

Signature: Mark F. Buchner
Date: December, 1991

IMPROVING NEUTRON DOSIMETRY USING BUBBLE DETECTOR TECHNOLOGY

A Thesis
Presented for the
Master of Science
Degree
The University of Tennessee, Knoxville

Mark Alan Buckner
December, 1991

To my Father and Mother, and loving memory of my Grandparents

ACKNOWLEDGEMENTS

Thanks be to the Majestic, Sovereign Creator and Sustainer of all things, the God of the Old and New Testament, who has endowed me with such abilities as seemed good in His sight, for the purpose of Glorifying and enjoying Him forever.

The author wishes to express his appreciation to the all individuals both silent and outspoken who have been a source of encouragement and assistance during his pursuit of this degree.

To T. A. Rhea: Thanks for the encouragement, instruction and provisional opportunities early on in my career. To C. S. Sims: Thank you for the patience, encouragement, and guidance both technical and spiritual. To Dr. L. F. Miller and Dr. P. Groer: I appreciate your comments, instruction and patience. To LtCmd Steve Doremus, of the U. S. Navy's Naval Dosimetry Center, Dr. Gordon Riel, of the Naval Surface Warfare Center, Dr. Martin Nelson and Dr. Mark Harper of the U. S. Naval Academy, Dr. W. H. Casson of Oak Ridge National Laboratory, Dr. H Ing of Bubble Technology Industries, Dr. R. E. Apfel of Apfel Enterprises, Dr. J. C. Liu of the Stanford Linear Accelerator Center and Dr. R. B. Schwartz of the National Institute of Standard and Technology: Thank you for your encouragement, guidance, and stimulating technical discussions. I eagerly anticipate future professional interaction with you all. To my family and friends: I thank God for you all! To David my true friend and brother; thanks for the encouragement and the council!

The author would also like to thank Dr. Joel Rabovsky and the Department of Energy's Office of Health for their encouragement and financial support of bubble detector research.

ABSTRACT

Providing accurate neutron dosimetry for a variety of neutron energy spectra is a formidable task for any dosimetry system. Unless something is known about the neutron spectrum prior to processing the dosimeter, the calculated dose may vary greatly from that actually encountered; that is until now. The entrance of bubble detector technology into the field of neutron dosimetry has eliminated the necessity of having an *a priori* knowledge of the neutron energy spectra. Recently, a new approach in measuring personnel neutron dose equivalent was developed at Oak Ridge National Laboratory. By using bubble detectors in combination with current thermoluminescent dosimeters (TLDs) as a Combination Personnel Neutron Dosimeter (CPND), not only is it possible to provide accurate dose equivalent results, but a simple four interval neutron energy spectrum is obtained as well. The components of the CPND are a Harshaw albedo TLD (two TLD-600/700 pairs one covered by cadmium, the other by ABS plastic) and two bubble detectors with theoretical energy thresholds of 100 keV and 1500 keV (BD-100R and BDS-1500 from Bubble Technology Industries, Canada).

The original CPND methodology has been modified with the goal of improving the spectrometric capabilities and the resulting dosimetric accuracy. The foci of the modification were:

- 1) refinement of the BD-100R and BDS-1500 response functions,
- 2) reevaluation of the TLD-600 thermal neutron sensitivity,
- 3) redefinition of the energy intervals for which the neutron spectrum is described, and
- 4) introduction of a matrix algorithm for neutron spectrum deconvolution and dosimetric determination.

The effectiveness of the modifications was assessed by reevaluating the original raw data from a series of radioisotopic source and *in situ* measurements and comparing

them with the original CPND results.

The results of the modified CPND demonstrate significant improvements in the spectrometric and dosimetric accuracy have been realized, relative to the original CPND characterization. This is evidenced by an overall increase in dosimetric accuracy of 2% for the *in situ* and 28% for the radioisotopic measurements. Individually, the modified version outperformed the original in eight of the ten measurements, while of the remaining two, one was the same and for the other the original results were better by 2%. The final neutron dose equivalent results were within 11% of the reference values for the five *in situ* spectra and within 2% of the reference values for the radioisotopic source spectra.

Presented are:

- 1) a synoptic history surrounding emergence of bubble detector technology,
- 2) a brief overview of the current theory on mechanisms of interaction,
- 3) the data and analysis process involved in refining the response functions,
- 4) performance evaluation of the original CPND and a reevaluation of the same data under the modified method as presented in this work,
- 5) the procedure used to determine the reference values of component fluence and dose equivalent for field assessments,
- 6) analysis of the after-modification results,
- 7) a critique of some currently held assumptions, offering some alternative explanations, and
- 8) my personal thoughts concerning potential applications and directions for future research.

Also provided in an appendix is a technical note detailing the organic nexus between the response characteristics of a neutron dosimeter, the fluence-to-dose equivalent factor and the neutron spectrum being measured, which includes several radioisotopic

source sensitivities and calibration factors calculated for the BD-100R and TLD-600.

TABLE OF CONTENTS

Chapter	Page
I INTRODUCTION	1
1.1 Necessity of accurate neutron dosimetry	1
1.2 Inherent difficulties associated with neutron dosimetry	2
1.3 Thesis structure	3
1.4 Advent of spectral information: threshold detectors	5
1.5 Bubble chamber	5
1.6 Bubble detector and superheated drop detector	6
1.7 Theory of interaction and bubble formation	8
1.8 Combination Personnel Neutron Dosimeter (CPND)	11
II IMPROVEMENT AND MODIFICATION OF THE CPND	13
2.1 Introduction and description of areas to be addressed	13
2.2 Refinement of the BD-100R and BDS-1500 R(E)s	14
2.3 Reevaluation of TLD-600 thermal neutron sensitivity	16
2.4 Redefinition of energy intervals (EI)	23
2.5 Matrix algorithm and spectrum deconvolution	26
2.6 Dose equivalent conversion	29
III PERFORMANCE EVALUATION AND ANALYSIS OF RESULTS	31
3.1 Introduction	31
3.2 Previous performance	32
3.3 Reassessment of reference spectra and dosimetric values	37
3.4 Performance reevaluation	38
3.5 Analysis of results	43
IV SOME ASSUMPTIONS AND ALTERNATIVE EXPLANATIONS	57
4.1 Useable lifetime	57
4.2 Response variation	58

4.3	Temperature affects and compensation methods	59
4.4	Bubble formation, growth and memory	64
V	FUTURE DIRECTIONS AND APPLICATIONS	73
5.1	Extremity dosimetry	73
5.2	Accident level dosimetry/spectrometry	73
5.3	A "do-it-yourself" bubble reader	76
5.4	Development of a Combination Area Neutron Spectrometer (CANS) .	79
5.5	Alternative Real-time Acoustical Processing (ARAP)	82
VI	SUMMARY AND CONCLUSIONS	86
	REFERENCES	90
	APPENDIX: The Spectral Nexus: Understanding the Relationship Between Response Functions and Neutron Spectra	95
	VITA	104

LIST OF FIGURES

	Page
Figure 2.2.1 TCC normalized data from mono-energetic irradiations and derived R(E)s for the BD-100R and BDS-1500	17
Figure 2.4.1 Step function: average sensitivity in neutron response per unit fluence	25
Figure 3.4.1 The relative accuracy of the CPND to measure neutron dose equivalent (H_{EI} and H_T) for ORNL <i>in situ</i> spectra at TRU	41
Figure 3.4.2 The relative accuracy of the CPND to measure neutron dose equivalent (H_{EI} and H_T) of RADCAL radioisotopic source spectra	42
Figure 3.4.3 Comparison of reference (BMS) and CPND measured spectrum for the glove box at TRU	45
Figure 3.4.4 Comparison of reference (BMS) and CPND measured spectrum for the cave area at TRU	46
Figure 3.4.5 Comparison of reference (BMS) and CPND measured spectrum for the control room at TRU	47
Figure 3.4.6 Comparison of reference (BMS) and CPND measured spectrum for the waste transfer area at TRU	48
Figure 3.4.7 Comparison of reference (BMS) and CPND measured spectrum for the analytical lab at TRU	49
Figure 3.4.8 Comparison of reference (BMS) and CPND measured spectrum for the $^{252}\text{Cf}(\text{PE})$ source at RADCAL	50
Figure 3.4.9 Comparison of reference and CPND measured spectrum for the $^{238}\text{PuBe}$ source at RADCAL	51

Figure 3.4.10	Comparison of reference and CPND measured spectrum for the $^{252}\text{Cf}(\text{D}_2\text{O})$ source RADCAL	52
Figure 3.4.11	Comparison of reference and CPND measured spectrum for a mixture of two RADCAL sources: $^{252}\text{Cf}(\text{D}_2\text{O})$ and $^{238}\text{PuBe}$ (MIX(2))	53
Figure 3.4.12	Comparison of reference and CPND measured spectrum for a mixture of three RADCAL sources: $^{252}\text{Cf}(\text{D}_2\text{O})$, $^{252}\text{Cf}(\text{PE})$ and $^{238}\text{PuBe}$ (MIX(3))	54
Figure 4.3.1	Phase diagram in the T,P plane	60
Figure 4.4.1	The life-cycle of a bubble	65
Figure 4.4.2	Correlative record of BD response and cumulative dose for a normal BD and one which contains bubbles that have exceeded the r_{cx}	69
Figure 4.4.3	PAG tension loss as a function of bubble growth	72
Figure 5.1.1	Experimental neutron extremity dosimeter (BUDEX)	74
Figure 5.3.1	A photograph of the do-it-yourself bubble reader	77
Figure 5.3.2	An image captured with the D-Y-I reader a) full image, b) magnified image	78
Figure 5.4.1	Description of the modified TLD component of CANS.	81
Figure 5.5.1	Real-time spectrometry: A) "pop" detected by a microphone; B) counted by simple circuitry and displayed; C) multiple detector signals come to a laptop with signal processing board, recorded, processed and spectral results displayed graphically	84
Figure 5.5.2	Real-time temperature corrected neutron dosimeter using a BD-100R and miniature ARAP	85
Figure A.1	The BD-100R R(E) and $^{241}\text{AmBe}$ and $^{252}\text{Cf}(\text{unmod})$ spectra normalized to 0.01 mSv	99

LIST OF TABLES

	Page
Table 2.3.1 Fluence distribution for TLD-600 sensitivity irradiations using $^{252}\text{Cf}(\text{D}_2\text{O})$ with and without the Cd shell.	21
Table 2.3.2 TLD-600 response to $^{252}\text{Cf}(\text{D}_2\text{O})$, with and without the Cd shell.	22
Table 2.3.3 TLD-600 sensitivities to incident and albedo thermal and epi-Cd neutrons.	22
Table 2.4.1 Original (Liu) CPND EIs, sensitivities and $h_\phi(\text{EIs})$	27
Table 2.4.2 Modified (New) CPND EIs, sensitivities and $h_\phi(\text{EIs})$	27
Table 3.2.1 The original (Liu) measured dose equivalent (H_{EI} and H_{T}) and measured divided by reference results from the radioisotopic source measurements	34
Table 3.2.2 The original (Liu) measured dose equivalent (H_{EI} and H_{T}) and measured divided by reference results from the <i>in situ</i> measurements at TRU.	35
Table 3.2.3 The individual bias and standard deviation of the original CPND for the radioisotopic measurements	35
Table 3.2.4 The individual bias and standard deviation of the original CPND for the <i>in situ</i> measurements	35
Table 3.2.5 The EI bias, standard deviation and L value of the original CPND for the radioisotopic and <i>in situ</i> categories	36
Table 3.3.1 Comparison of original (Liu) and modified (New) reference values for radioisotopic source neutron H_{EI} and H_{T} measurements.	38

Table 3.3.2	Comparison of original (Liu) and modified (New) reference values for the neutron H_{EI} and H_T TRU <i>in situ</i> measurements.	39
Table 3.4.1	The modified (New) measured dose equivalent (H_{EI} and H_T) and measured divided by reference results from the radioisotopic source measurements	39
Table 3.4.2	The modified (New) measured dose equivalent (H_{EI} and H_T) and measured divided by reference results from the <i>in situ</i> measurements at TRU.	40
Table 3.4.3	The individual bias and standard deviation of the modified CPND for the radioisotopic measurements	40
Table 3.4.4	The individual bias and standard deviation of the modified CPND for the <i>in situ</i> measurements	41
Table 3.4.5	The overall bias, standard deviation and L value of the modified CPND for the radioisotopic and <i>in situ</i> categories	41
Table 3.5.1	Comparison of the original and the modified overall performance indicators	54
Table 4.4.1	Theoretical response of two bubble detectors before and after acquiring three bubbles exceeding r_{cx}	?
Table A.1	Calculated values of $\bar{E}(\phi)$, $\bar{E}(H)$, \bar{h}_ϕ and BD-100R response for several radioisotopic neutron sources	101

NOMENCLATURE

English Symbols

ARAP	Alternative Real-time Acoustical Processing
BD	bubble detector
CPND	Combination Personnel Neutron Dosimeter
EI	energy interval
H	dose equivalent
h_d	fluence-to-dose equivalent conversion factor
PAG	polyacrylamide gel
R(E)	response function
TLD	thermoluminescent dosimeter

Subscripts

b	bubble
c	critical
cx	critical expansion
fx	critical formation
t	thermal
m	medium
s	slow
f	fast
EI	energy interval
T	total

Greek symbols

ϕ	fluence
Φ	flux
σ	surface tension
Θ	scattering angle of the neutron in the center-of-mass system
θ	scattering angle of the recoil nucleus in the lab coordinate system

PROLEGOMENON

As a pursuant of the noble degree of Master of Science it behooves me to seriously acknowledge the heights to which I must attain to live up to this high calling. And a high calling it is indeed; for great have been those who have gone before us, those to whom we owe so much of that which we call science - being derived from the latin *scientia* which means knowledge. And at the onset, we must humbly confess that the attainment of knowledge is grounded upon certain presuppositions. The pursuit itself presupposes an object that is knowable, i.e., the elements and the inter-relationships between these elements, a self-conscious subject, and that an organic relation exists between the two. The acquiescence of knowledge presupposes that some knowledge about the object is communicable, that it is capable of being accurately transmitted, that a reliable means of communication exists between the object and the subject, and that the subject is predisposed to perceive this communication.

The very notion that the subject embraces this perception as valid and truthful presupposes faith; for there is no absolute empirical method for verifying the veracity of this communication any more than there is of proving the existence of one's self, other than by an awareness of one's own consciousness; even this self-consciousness is of itself a fruit of faith. Yet, perception in and of itself is not knowledge rightly called; for the perception must then be taken up into the consciousness of the subject, where, by the faculty of reason, the elements observed and the relationships that exist between these elements are elevated to become a subjective, derived, knowledge of the object. Therefore, knowledge, which is the essence of science, is the cognizance of the elements and the relationships between these elements as they truly exist within the object of our science. As a result all true knowledge is merely an assimilation and restatement of the things as they truly are within the object; correspondingly, there exists no knowledge (unless falsely called) that does not coincide with an original archetypal knowledge, and no true scientist (unless falsely

called) that does not meticulously study the "organic world of thought that lies in the cosmos, until his own world of thought entirely corresponds to it" (Kuyper 1980).

All men hold presuppositions. The only question is: who holds the right presuppositions? The only true presupposition, and the one that I hold as my basis for science and all of life, is the self-existent eternal triune God of the Bible, who has revealed Himself in nature, and within man's consciousness, but most clearly in scripture. He has told us that He designed and created, from nothing, all that is, whether visible or invisible, by His spoken fiat; according to His plan, and for His purpose, He called into being, and continues to sustain, all the elements and all the relationships existing between these elements, i.e., the object of our science. Admittedly this presuppositional stance is both old and uniquely Christian, but, for centuries, it was the foundational basis for western scientific endeavor. Consider the stated purpose of Harvard College, founded in 1636: "Let every student be plainly instructed, and earnestly pressed to consider well, the main end of his life and studies is, to know God and Jesus Christ which is eternal life (John 17:3) and therefore lay Christ at the bottom, as the only foundation of all sound knowledge and learning" (DeMar 1990).

Every so called fact of the cosmos is, by design, revelatory of God. "Scripture tells us that God, the God who has more fully revealed Himself in scripture than in nature, is yet speaking to us in the created universe about us. Scripture says that *from the beginning* He has spoken there. It says that man has known this fact, and that by his efforts at perversion he has well-nigh succeeded in silencing the voice of revelation, but deep in his heart he is still aware of this revelation and will be held responsible for it" (Van Til 1972). As man looks upon the created cosmos he thinks about it. As he thinks about it, he interprets it. At this point of interpretation, which of itself is also revelatory of God, man is morally obligated to interpret it as God has said that it is. Yet man has suppressed, and continues to suppress this truth. He does so in failing to acknowledge God as God, denying that it was this self-revealing God who created man himself and the cosmos about him, and has given him the task of cultivating and keeping it. Professing to be sufficient unto himself, would-be

autonomous man expresses no thanks to this God who sustains his life and blesses him with innumerable goods. Claiming to be the father of his own destiny, he ignores God, factoring Him out of the interpretation of life and science all together. He defines the rules which govern nature as natural laws, instead of God's laws, and the elements of the cosmos as brute facts, instead of God-created facts. He becomes proud and arrogant, boasting of "his" many accomplishments and technological advances. "Two Creators, one real, the other would-be, stand in mortal combat against one another; the self-contained triune God of Christianity and the *homo noumenen*, the autonomous man of Immanuel Kant, cannot both be ultimate" (Van Til 1972). But this self-acclaimed autonomy, this act of ignoring God, is a sin in sight of the God who has told us that whether we eat or drink, or whatsoever we do, we are to do all to His Glory!

He is Truth!; it is because His knowledge is comprehensive and exhaustive and that He reveals a part of His knowledge to man, that we as scientists can truly "know" anything at all. "In Thy light we see light" (Psalm 36:10). So then, it is upon the presupposition of the ontological Trinity that I endeavor to pursue knowledge, confessing that I, as all lovers of *scientia*, merely "think God's thoughts after Him!"

To God be the Glory!

Chapter I

INTRODUCTION

A proposed increase in neutron quality factor and reduction of the annual dose equivalent limits for radiation workers; harbingers indeed! Amidst the already numerous difficulties associated with performing neutron dosimetry these magnify the need to increase the accuracy and precision of our methods.

1.1 NECESSITY OF ACCURATE NEUTRON DOSIMETRY

We are at a critical juncture in Department of Energy (DOE) history. With the recent growth of activities aimed at ensuring the adherence of facilities utilizing nuclear grade material to the stringent guidelines required by the Occupational Safety and Health Administration (OSHA), Environmental Protection Agency (EPA), Nuclear Regulatory Commission (NRC) and DOE, the current prospect of increasing the neutron quality factor, DOE's ongoing investigation into the plausibility of decreasing the annual dose equivalent limits, and emphasis on maintaining personnel exposures as low as reasonably achievable (ALARA), never has there existed a greater necessity to "monitor to the max". These prevailing winds of change necessitate a major reform of dosimetry as we know it. We will be required to run harder than before to stay in the same place.

Until recently, organizations would have been hard pressed to find an affordable neutron monitoring system capable of surmounting the inherent difficulties associated with routine neutron dosimetry in multiple spectral environments, not to mention these rigid demands lurking on the horizon. The exigency of the situation necessitates a serious look at the current status of neutron dosimetry.

1.2 INHERENT DIFFICULTIES ASSOCIATED WITH NEUTRON DOSIMETRY

Performing good personnel neutron dosimetry, with the current technology, requires:

- 1) an in-depth understanding of the energy response characteristics of the dosimeter utilized,
- 2) fluence-to-dose equivalent conversion methodologies,
- 3) a cognizance of the calibration procedure and sources used,
- 4) an *a priori* knowledge of the neutron spectrum in the areas monitored, and
- 5) the calibration factors required to correct for variations in the field including differences between field and calibration spectra.

The perfect routine neutron dosimeter would provide an accurate assessment of the dose equivalent received by the individual being monitored without the application of correction factors.

To my knowledge, all current personnel neutron dosimetry systems are dependent upon some knowledge of the neutron energy spectra prior to assessment of the neutron dose equivalent. Whether it be from Bonner multi-sphere (BMS) measurements or 9-to-3 inch ratios, unless something is known about the neutron spectrum prior to processing the dosimeter, the calculated neutron dose equivalent (H_n) could vary greatly from that actually encountered. That is until now!

The recent introduction of bubble detector technology has made navigable waters previously uncharted in the history of neutron dosimetry. It is now possible to provide an accurate measurement of neutron working environments without an *a priori* knowledge of the neutron spectrum. This is attainable through the use of the Combination Personnel Neutron Dosimeter (CPND). The CPND measures neutron fluence (a real quantity) and reports it by virtue of a simple four interval spectrum. This fluence measurement is the basis for determining the neutron dose equivalent.

1.3 THESIS STRUCTURE

The dissertation of Liu stated that "... the CPND was designed to be superior to present neutron dosimeters in that it will have crude neutron spectrometric capability..." (Liu et al. 89). After an in-depth and critical analysis of the work surrounding development and evaluation of the CPND, it was believed that (with some refinement) the demonstrated performance of the CPND to measure neutron dose equivalent for a variety of neutron spectra (both radioisotopic and *in situ*) could be made even better.

The remaining sections of Chapter I address the foundational work upon which bubble detector technology was erected. This includes the current status of the technology, a thumbnail sketch of the currently held beliefs on the mechanisms involved in bubble formation and an introductory description of the CPND.

Chapter II describes the features of the CPND which were modified and the reasoning behind them. These include:

- 1) refinement of the BD-100R and BDS-1500 response functions,
- 2) reevaluation of the thermal neutron sensitivity of TLD-600 (because the use of albedo TLD is prolific and information is available in abundant measure, little supporting information is provided),
- 3) redefinition of the energy intervals (EI) used to describe the spectra,
- 4) development of a spectrum deconvolution matrix algorithm, and
- 5) the final neutron dose equivalent determination.

The effectiveness of these modifications in enhancing the spectrometric capabilities and in improving the overall neutron dose equivalent accuracy was assessed by comparing the original raw data processed according to the modified methodology to the original results and to reference dosimetry. A condensed version of the original results (as well as a presentation and analysis of the results after modification) are described in Chapter III. The redefinition of the energy intervals (EI) required that reference dosimetry be redetermined to correspond with the newly

defined EIs. The method and redefined reference dosimetry are included in this chapter.

A more theoretical direction is taken in Chapter IV where some currently held beliefs surrounding the bubble detector are addressed. A critique and some alternative explanations about:

- 1) useable lifetime,
- 2) observed response variations,
- 3) temperature affects,
- 4) bubble growth,
- 5) bubble memory,
- 6) incompressible bubbles, and
- 7) theory of operation are provided.

Chapter V takes a look at some suggested research and potential applications of bubble detector technology for:

- 1) extremity dosimetry,
- 2) accident level dosimetry,
- 3) a do-it-yourself bubble reader for research applications,
- 4) a Combination Area Neutron Spectrometer (CANS), and
- 5) a different approach to bubble detection which is currently under development in the Dosimetry Application Research Group (DOSAR), Alternative Real-time Acoustical Processing (ARAP).

A summary statement and closing remarks are to presented in Chapter 6.

Additional knowledge gained from this research is described in Appendix 1 under the title of "The Spectral Nexus: Understanding the Relationship Between Response Functions and Neutron Spectra". This addresses:

- 1) some of the pitfalls associated with the common practice of describing a neutron spectrum by the average energy,
- 2) the expected variation in response of the BD-100R and TLD-600 for several radioisotopic source spectra (based on a folding

of the response functions into a reference spectrum for each source),

- 3) the derived source specific sensitivities, and
- 4) a correction methodology.

Let us now take a brief look at the emergence of spectral investigation and the coming-of-age of the bubble detector.

1.4 ADVENT OF SPECTRAL INFORMATION: THRESHOLD DETECTORS

G. S. Hurst recognized in 1956 that knowledge of the neutron spectrum is essential for accurate tissue dose determination (Hurst et al. 1956). He introduced a method for measuring the spectrum of fast neutrons utilizing a series of activation foils. By creatively combining activations foils of differing energy thresholds and changing the shielding configurations (five detectors total), he was able to deconvolute a crude five interval neutron spectrum. This device became appropriately known as the threshold detection unit or TDU.

1.5 BUBBLE CHAMBER

Glasser discovered in 1952 that some liquids become radiosensitive while in a superheated or metastable state (Glasser 1952). A superheated or metastable state could be obtained by lowering the pressure of a chamber containing a liquid below the vapor pressure of that liquid. Tracks of bubbles are created in the bubble chamber by the incident radiation. Equilibrium is reestablished within the chamber by applying pressure sufficient enough to recompress the gas, transferring it back to the liquid phase. Lowering the applied pressure superheats the liquid, rendering it once again sensitive and ready for detection. The difficulties associated with sustaining a liquid in a superheated state are that the "live time" rarely exceeded a few minutes and that the bubble chamber detects single events (the tracks of a single ion). These have impeded the use of the bubble chamber for neutron dosimetry or spectroscopy. The theory explaining bubble formation has become known as Seitz's thermal spike model, i.e., the vaporization of a superheated liquid by ionizing or

secondary charged particles (Seitz 1958).

1.6 BUBBLE DETECTOR (BD) OR SUPERHEATED DROP DETECTOR (SDD)

Apfel continued the study of radiation-induced acoustic cavitation begun by Liberman, Finch, Hahn, Peacock, West, and Howlet, with his study of "superheated droplets rising in a heated 'host' liquid". He discovered that the superheated state of liquid could be sustained for longer periods by isolating the liquid into droplets (Apfel 1979).

Recently, two hybrid neutron detectors have emerged which capitalize on the suspension of a superheated liquid (SHL) in a host medium. One is the superheated drop detector (SDD) of Apfel Enterprises (Æ) (SDD is a trademark of Apfel Enterprises, Inc., 25 Science Park, New Haven, CT 06511.) and the other is the Bubble-damage Detector (BD) of Ing's Bubble Technology Industries (BTI). Each utilizes its own unique design and detection philosophy. Both isolate individual droplets of SHL by dispersing them throughout a holding medium. This medium acts to isolate the droplets and to increase the tensile strength properties of the liquid. The result is a detector composed of many tiny bubble chambers. This isolation removes the necessity of recompression after detection of a single event, and it maintains the droplets in a superheated state nearly indefinitely (when compared to the bubble chamber), and it facilitates the detection of multiple events integrated over time. Although both designs employ differing methodologies for isolating the SHL droplets and for quantifying the bubbles after formation, in principle, their genesis is traceable to Glasser's bubble chamber, Seitz's thermal spike model and cavitation theory.

BTI and post-event detection

The BTI detector is built upon a passive *a posteriori* concept. The SHL droplets are suspended in a transparent elastic polyacrylamide gel (PAG). Once a droplet is vaporized the PAG entombs or immobilizes the bubble at the site of

formation, enabling it to be counted after growing to a visible size.

The sensitivity of the BD may be controlled by changing the density or number of droplets per unit volume in the detector. Detectors with differing neutron energy thresholds have been made possible by manipulating the composition of the SHL and by altering the medium composition. A typical SHL droplet (prior to vaporization) is approximately 25 μm in diameter. Immediately after vaporization a bubble is approximately 1-2 mm and may be seen by the unaided eye (Liu 1989). A new generation of bubble detectors with droplet sizes which are significantly smaller than the standard detector has been manufactured by BTI . These μ -bubble detectors require magnification or a 24 hour growing period before they can be easily read.

A semiautomatic reader capable of reading both the standard and μ -droplet devices is available from BTI. The second generation reader will store the count information along with the detector number (entered by the operator). It will also report the dose equivalent when using the BD-100R (a nearly dose equivalent detector).

Apfel and active detection

An *ad hoc* approach to bubble detection is taken by \mathcal{A} . Because the microscopic drops of SHL are suspended in a viscous gel, neutron interactions may be detected by measuring 1) the gas volume evolving from the formed bubbles or 2) the number of acoustical sound waves or "pops" emitted during bubble formation. The first method is used with the Neutrometer. The Neutrometer resembles a piece of thin glass tubing filled with SHL mixture. A disc floats on the surface of the SHL mixture. As bubbles are formed, the evolved gas displaces the SHL mixture and the disc rises in the tube. The dose equivalent may be determined by correlating the position of the disc and the graduated scale on the side of the device. In the second method, a transducer or microphone is placed in proximity of a vial containing the SHL mixture. A small microprocessor records the number of acoustical "pops" and translates this information into neutron dose equivalent. The microprocessor could also correct for depletion of the SHL and temperature dependence and apply a

correction factor to account for differences between the field and the calibration spectra. Detailed information on the theory and design of both these devices is available in the open literature (Roy et al. 1987; Ing 1984).

1.7 THEORY OF INTERACTION AND BUBBLE FORMATION

In order to understand the complex transformation process from incident neutron to bubble, a knowledge of several different areas of science is required. The physical process encompasses the domains of:

- 1) nuclear physics (ion production via neutron-nucleus interaction),
- 2) atomic physics (ionic interaction with matter), and
- 3) fluids and thermodynamics (bubble formation via vaporization)

(Roy et al, 1987).

Is it any wonder that no model currently exists which comprehensively predicts bubble formation?

The following is a condensed summary of the major components constituting the currently accepted explanation for bubble formation, cavitation theory.

Ion Production

The first stage in the process is ion production by a nonionizing neutron. The primary mechanism responsible for this initial phase is the interaction of the incident neutron with the nucleus of an atom by means of a simple billiard-ball type elastic scatter.

The conservation of energy and momentum in the center-of-mass system (COM), define the relationship between the energy of a recoil nucleus in (E_R in the laboratory coordinate system (LCS)) and the kinetic energy of the incoming neutron (E_n in LCS) and the scatter angle of the recoil neutron θ (COM),

$$E_R = \frac{2A}{(1+A)^2} (1 - \cos\theta) E_n, \quad (1.7.1)$$

where

$A = \text{mass of target nucleus} / \text{neutron mass}.$

The following association is made between the scattering angle of the recoil neutron Θ , in the COM, and the scattering angle of the recoil nucleus θ , in the LCS,

$$\cos \theta = \sqrt{\frac{1 - \cos \Theta}{2}}. \quad (1.7.2)$$

Solving for $\cos \theta$ and substituting it into Equation (1.7.1), Equation (1.7.2) simplifies to relate the energy of the recoil nucleus in terms of its own recoil angle,

$$E_R = \frac{4A}{(1+A)^2} (\cos^2 \theta) E_n. \quad (1.7.3)$$

From this we see that a distribution of E_R from zero, for a slightly grazing encounter ($\theta = 90^\circ$), to a maximum, in the event of a head-on collision of ($\theta = 0^\circ$), will occur when all recoil angles are possible.

By defining $\sigma(\Theta)$ as the differential scattering cross section of the neutron in the COM and σ_s as the total scatter cross section integrated over all angles, the probability of a recoil ion of energy E_R ($P(E_R)$) can be calculated by,

$$P(E_r) = \frac{(1+A)^2}{A} \times \frac{\sigma(\Theta)}{\sigma_s} \times \frac{\pi}{E_n}, \quad (1.7.4)$$

(Knoll 1979). Equation 1.7.4 shows that the expected distribution of the energy continuum of the recoil ion will mimic that of the $\sigma(\Theta)$. The shape of the $\sigma(\Theta)$ will favor forward scattering for most nuclei.

Energy Transfer

After the energy is transferred to a recoil nucleus, the charged nucleus deposits its energy by interaction with electrons and other nuclei via ionization and excitation.

Bubble Formation

According to Seitz's thermal spike model, ionization and excitation along the charged particle track induces heat which causes the SHL to vaporize or nucleate (Seitz 1958). Apfel offers an explanation for this nucleation or bubble formation known as cavitation or nucleation theory that incorporates Seitz's "thermal spike" model. (Apfel 1979 & 1987).

According to Roy (Roy et al. 1987), once a bubble of radius r is formed, it will continue to exist in a stable state as long as the pressure within the bubble remains equal to the pressure exerted on the bubble from without. This was described by him as the effective surface pressure,

$$P_{es} = \frac{2\gamma(T)}{r}. \quad (1.7.5)$$

This equation may be rewritten in terms of the pressure differences ΔP within and without the bubble,

$$\Delta P = P_v(T) - P_0 = \frac{2\gamma(T)}{r_c}, \quad (1.7.6)$$

where $P_v(T)$ is the vapor pressure within the droplet at temperature T , and $\gamma(T)$ is the surface tension of the liquid at temperature T . Solving Equation 1.7.6 for r_c we obtain,

$$r_c = \frac{2\gamma(T)}{\Delta P}. \quad (1.7.7)$$

This equation indicates that if a bubble grows to a size where its radius is as large as or exceeds r_c the bubble becomes thermodynamically unstable and it will continue to grow by consuming or boiling the entire SHL droplet. Thus r_c is defined as the critical radius. According to Seitz, the minimum energy required to form a bubble of r_c is provided by charged recoil particles from neutron interactions (Seitz 1958). Restated, the critical radius is the point at which the growing bubble becomes thermodynamically unstable, and it overcomes the surface tension of the liquid, the effective atmospheric pressure and the surface tension of the holding medium. At this point it boils violently and emits an acoustical shockwave or acoustic pressure pulse (Roy et al. 1987). This bubble will continue to grow until equilibrium is reestablished between the vapor pressure within the newly formed bubble, $P_v(T)$, and the external pressure, P_0 .

The energy required to form a spherical bubble of radius r is described by the free energy equations for surface free energy, vaporization and expansion (Roy et al. 1987).

1.8 COMBINATION PERSONNEL NEUTRON DOSIMETER (CPND)

In 1989 C. J. Liu, led by information gathered from a review of current methods for neutron dosimetry, developed the Combination Personnel Neutron Dosimeter (CPND) at Oak Ridge National Laboratory (ORNL). The concept of the CPND is very similar to that employed in the TDU, i.e., the use of multiple detectors with differing thresholds to provide a simple neutron spectrum. The difference between the TDU and the CPND is that the CPND uses bubble detectors and albedo thermoluminescent dosimeters (TLD) instead of activation foils. The BD-100R and BDS-1500, which possess theoretical thresholds of 100 and 1500 keV, and the Harshaw albedo TLD used by Martin Marietta Energy Systems (MMES) are the elements of the CPND. The goal of the CPND is to provide an accurate measure of neutron dose equivalent by measuring the neutron spectrum contributing the dose equivalent. This becomes increasingly desirable considering the current

recommended change of the neutron quality factor. Since fluence is a real quantity, if the spectrum is known, the neutron dose equivalent can be determined by applying the appropriate fluence-to-dose equivalent conversion factors (h_p s).

Chapter II

IMPROVEMENT AND MODIFICATION OF THE CPND

The "proof is in the pudding" so to speak, and the CPND has demonstrated its efficiency by providing an accurate measure of both dose equivalent and neutron spectrum for ten neutron fields, five radioisotopic and five *in situ* environments at ORNL. Yet, even these good results can be improved by making a few modifications. A description of these modifications is provided.

2.1 INTRODUCTION AND DESCRIPTION OF AREAS TO BE ADDRESSED

Since the completion of Liu's dissertation, BD research has continued at ORNL as a joint venture with the Naval Surface Warfare Center (NSWC), Naval Research Laboratory (NRL), United States Naval Academy (USNA), and National Institute of Standards and Technology (NIST) with financial support from the Department of Energy (DOE). The additional information obtained from this collaboration was instrumental in achieving the desired modifications.

The modifications consisted of:

- 1) refining the energy response characteristics of the BD-100R and BDS-1500,
- 2) a reevaluation of the accepted thermal neutron sensitivity of the TLD-600 elements of the CPND,
- 3) redefining the energy intervals, and
- 4) development of a matrix based spectrum deconvolution algorithm.

2.2 REFINEMENT OF THE BD-100R AND BDS-1500 R(E)S

The failure to establish an efficient method of collecting and maintaining data at the inception of a project often impedes future development and direction. Prior to this work, data collected from the evaluation and testing of bubble dosimeters had been retained by the individuals performing the various tests. Though the need for an individual to collect and manage the data was recognized early in the project, for various reasons no one was given the responsibility. The decision was made at the January 1990 Bubble Dosimeter Working Group Meeting that the DOSAR group would head up this task. In May of the same year action began on compiling the data and standardizing a method for data entry and retrieval.

DOSAR developed a data base in which the entire contents of the BD research coalition was amassed. This amalgamation of data constituted the largest single quantity of information on BD research to date.

Monoenergetic irradiations

Included in this data were the results from a series of monoenergetic irradiations performed at the National Physical Laboratory (NPL) in England and a similar series of irradiations conducted at Pacific Northwest Laboratory (PNL) and the NIST reactor in the United States. Monoenergetic neutrons were obtained via scatter reactions at the Van de Graaff accelerators of NPL and PNL and three filtered reactor beams at NIST. The accelerator scatter-beams generated neutrons of 0.1, 0.25, 0.565, 1.2, 2.6, 3.2, 5.0, and 14.8 MeV, and the three reactor beams were at 2, 24, and 144 keV. Liu conducted the irradiations at PNL (Liu 1989), and Schwartz conducted them at NPL (Schwartz and Hunt 1990).

Because: 1) the detectors in both studies were not identical in sensitivity, 2) a constant temperature was not maintained for all the irradiations, and 3) different data recording methods were used, manipulation of the data was necessary. This was performed to establish a correlation between the two individual studies and to produce a reference point for further analysis.

Normalizing the Data

The BDs varied in sensitivity from 0.75 to 3.5 bubbles per 0.01 mSv (bu/mrem); therefore, the tube correction coefficient (TCC), defined as the reciprocal of the manufacturers sensitivity as found on the detector, was introduced as a means of normalizing the data. This approach mimics the element correct coefficient method employed for TLDs, i.e.,

$$R_i = TCC * R_0, \quad (2.2.1)$$

where

R_i = response normalized to 1 bu/0.01 mSv (mrem⁻¹),

TCC = tube correction coefficient, 1 / (sensitivity on detector i.e. 0.01 mSv/bu), and

R_0 = initial raw response of the detector (number of bu).

Thus, the result of each detector was normalized to reflect the anticipated response of a 1 bu per 0.01 mSv detector by multiplying the raw data by its respective TCC.

Temperature Correction

Because variations in ambient temperature are known to effect detector response (Ing and Birnboim 1984) and because a constant temperature was not maintained for all irradiations, initial temperature corrections were assumed based on the proportional relationship between temperature, volume, and pressure (i.e., $PV = kT$). According to Equations 1.7.1 and 1.7.2, the related effect on the superheatedness of the SHL and therefore the r_c is given by,

$$R_c = (T_0/T_c) * R_p, \quad (2.2.2)$$

where

- R_c = response after temperature correction,
 T_o = 20°C,
 T_e = temperature in °C at time of exposure, and
 R_i = initial response normalized to 1 bu per 0.01 mSv.

The R(E)s for the BD-100R and BDS-1500 were derived from curve fits to these normalized data.

Because the detector sensitivities provided by BTI, in bubbles per mSv, were based on calibration to the $^{239}\text{PuBe}$ source at Chalk River (Ing 1991), these derived R(E)s were normalized to yield a response of 1 bu per 0.01 mSv when exposed to a $^{239}\text{PuBe}$ spectrum. In essence, this R(E) is taken to be the true representation of a 1 bu per 0.01 mSv, 20°C, $^{239}\text{PuBe}$ calibrated BTI detector. The normalized data and the R(E)s are shown in Fig. 2.2.1.

2.3 REEVALUATION OF THE TLD-600 THERMAL NEUTRON SENSITIVITY

There are several factors which affect the response of a TLD-600 albedo-based dosimeter. Some of the pertinent considerations include:

- 1) the distance from the detector to the phantom or body,
- 2) the number, thickness, and dopants in the crystal,
- 3) the configuration and thickness of the thermal neutron absorbing filters (typically, cadmium (Cd) or boron (^{10}B)),
- 4) the heating methodology and profile employed to read the TLD, and
- 5) the encapsulation material, if applicable, (glass, teflon or bare chip).

Some of the different heating methodologies are: planchet, hot-finger, thermoelectric, laser, and hot-gas. Several stages of the heating profile may be altered; pre-heating conditions, heating ramp rate (in degrees per unit time), the maximum temperature, and the holding and the anneal times, are a few.

Consequentially, before inferences may be made from one type of

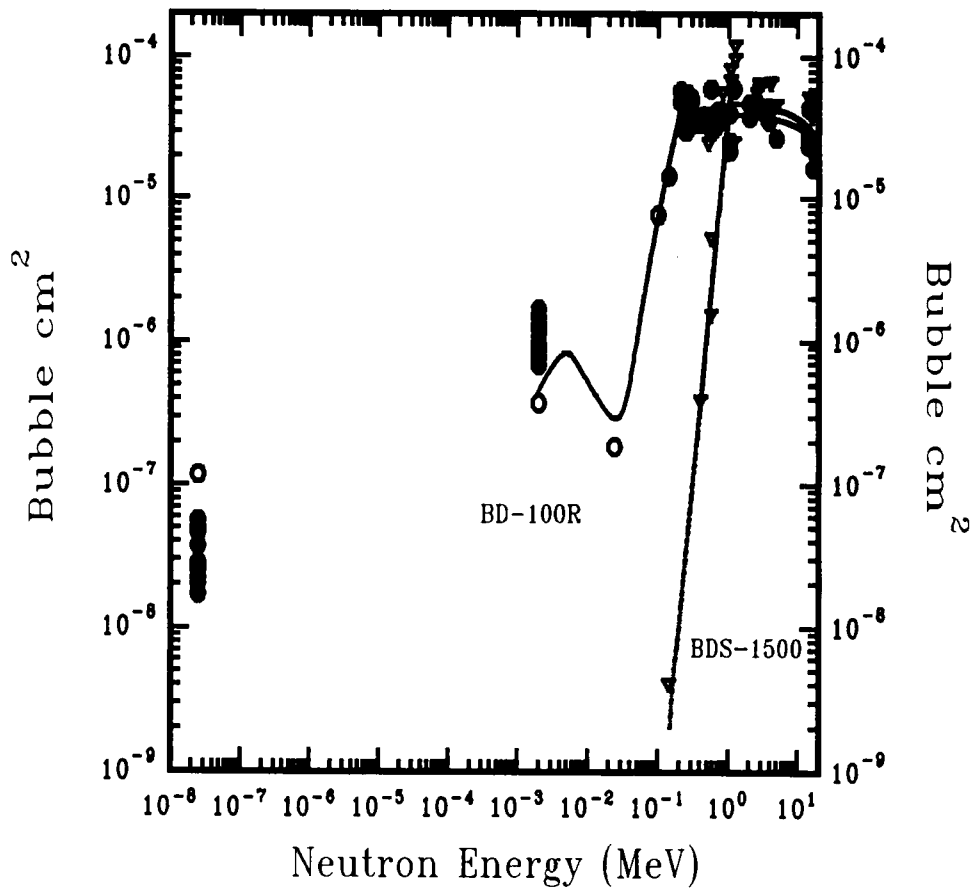


Fig. 2.2.1 The TCC normalized data from mono-energetic irradiations and derived response functions, $R(E)$, for the BD-100R and BDS-1500.

configuration or heating profile to another, these differences should be carefully weighed and appropriate assumptions must be drawn.

It is my opinion that Liu made some incorrect assumptions in the previous determination of the thermal neutron sensitivity of the Cd covered TLD-600 chip. These assumptions affect the appropriateness and accuracy of the measurements derived by this component of the CPND and consequently the performance of the CPND itself.

Liu derived the sensitivities of the TLD-600 elements of the CPND from the methodology espoused by Alsmiller (Alsmiller and Barish 1974). As I interpret it, in order for Liu to have come to his conclusions regarding the thermal neutron sensitivities of the TLD-600 elements the following assumptions must have been held, either consciously or unconsciously. Noted; not all of these points are necessarily disjoint from one other. As I interpret them the assumptions are:

- 1) "the Cd covered TLD-600 detects only albedo thermal neutrons" (Liu 1989),
- 2) the thermal-albedo of incident neutrons above 0.414 eV is negligible,
- 3) the response of the Cd-covered TLD-600 is due to incident thermal neutrons which are reflected, which according to Fig. 2 of Alsmiller is 0.8,
- 4) applying a ratio of the relative response at known energies to the relative response at thermal energies, derived from Fig. 3 of Alsmiller, to the data obtained from monoenergetic neutron irradiations, is adequate for determining the thermal neutron sensitivity of the Cd-covered TLD-600, and
- 5) that dividing the derived thermal neutron sensitivity of the Cd-covered TLD-600 by "the albedo factor of 0.8 for thermal neutrons" is adequate for determining the thermal neutron sensitivity of the plastic covered TLD-600 (Liu 1989).

In my opinion, the method employed by Liu to determine the thermal neutron

sensitivity of the TLD component of the CPND is incorrect. The Alsmiller data referenced by Liu, were derived from a one-dimensional discrete ordinate code using a 30-cm-thick semi-infinite tissue slab, and not TLD-600. The data in Fig. 2 of Alsmiller and Barish describes the "albedo-neutron fluence integrated over the specified energy ranges verses incident neutron energy for monoenergetic neutrons" (Alsmiller and Barish 1974). Figure 3 depicts the "relationship between the thermal albedo-neutron fluence and the dose equivalent produced in the tissue slab" (Alsmiller and Barish 1974). Liu bases the sensitivity of the Cd-covered TLD-600 on the ratio of the relative thermal neutron sensitivity to that at higher energies derived from Fig. 3. In so doing, he failed to recognize the disparity between the fraction of incident thermal neutrons which strike the phantom in the Alsmiller and Barish model as compared to the Cd-covered TLD-600 of the CPND. The relative thermal neutron sensitivity in Fig. 3 assumes that 100% of the incident thermal neutrons strike the slab, and that 0.8 of them are reflected. Although this is true for the Alsmiller model, it is not true of the Cd-covered TLD-600 in the CPND. The Cd-cover "absorbs 99.5% of the incident thermal neutrons" (Liu 1989). This alone would suggest that obtaining thermal neutron sensitivities for the CPND's Cd-covered TLD-600, by applying ratios derived from Fig. 3, will be in error. And, although the TLD-600 sensitivity to incident neutrons above 0.414 eV is considerably lower than it is for thermal neutrons, according to Fig. 2 of Alsmiller, 45% of the incident neutrons from 0.414 eV - 0.1 keV are reflected as thermal neutrons. Liu states that the Cd-covered TLD-600 detects only albedo thermal neutrons. Thus, his determination of thermal neutron sensitivity of the Cd-cover TLD-600, using ratios derived from Fig. 3 of Alsmiller, indicates that he also failed to consider the portion of the Cd-covered TLD-600 response that is attributable to the incident neutrons above 0.414 eV which are reflected at thermal energies. Consequently, the incident thermal neutron sensitivity he derived includes the sensitivity to incident neutrons of higher energies as well. These errors suggest that the true sensitivity of the Cd-covered TLD-600 to incident thermal neutrons is less than the 14.7×10^{-5} mR cm² stated by Liu.

Liu then proceeds to determine the thermal neutron sensitivity of the plastic

covered TLD-600 by dividing the Cd-covered sensitivity by the albedo factor of 0.8 obtained from Fig. 2 of Alsmiller. There are two errors associated with this procedure. First, as stated previously, application of the 0.8 albedo factor requires that 100% of the incident thermal neutrons strike the slab in order for 0.8 to be reflected, and this is not true for the Cd-covered TLD-600. Second, because the thermal neutron sensitivity of Cd-covered TLD-600 was overestimated, the derived thermal sensitivity of the plastic-covered TLD-600 would also be an overestimate. Therefore, based on these statements, I conclude that the actual thermal neutron sensitivities of both TLD-600 elements are lower than those stated by Liu. These overestimates will promulgate errors in the CPND's spectrometric measurements. Consequently, the derivation of more accurate thermal neutron sensitivities should improve the spectrometric accuracy of the CPND.

A more desirable method for correctly ascertaining the thermal neutron sensitivity of the TLD-600 elements would have to conduct measurements in a calibrated thermal neutron beam. But since this was not possible, an alternative method was employed. A series of experiments was conducted exposing the TLDs on phantom and in air to $^{252}\text{Cf}(\text{D}_2\text{O})$ with and without the Cd shell on the D_2O filled sphere. The emission of the ^{252}Cf source at the time of irradiation was determined from the NIST certificate emission on 4/30/87 by adjusting for decay using a half-life of 2.64 years using,

$$E_t = E_0 \times e^{-\frac{0.693 \times t}{T_{1/2}}}, \quad (2.3.1)$$

where

E_t = emission on date of interest,

E_0 = emission on date of calibration,

t = time, in years, since calibration, and

$R_{1/2}$ = half-life of source, in years.

The fluence at 0.5 m (the point of irradiation) was calculated for the irradiation with the Cd shell using,

$$\phi_r = \frac{E_i \times t}{4 \pi r^2}, \quad (2.3.2)$$

where

E_i = source emission ($\text{cm}^{-2} \text{ sec}$),

t = duration of irradiation (sec), and

r = distance from centerline of source (cm).

Air and room scatter values were calculated using the methodology described in (Eisenhauer et al. 1985). The reduction in the total neutron fluence that occurs by adding the Cd shell is effected by the absorption of neutrons below the Cd cutoff of 0.414 eV i.e., the absorption of thermal neutrons, and is calculated by (Eisenhauer 1984),

$$\phi_t = 0.115 \times \phi_T \quad (2.3.3)$$

where

ϕ_t = thermal fluence, and

ϕ_T = total fluence.

Thus, the difference in fluence between the irradiations with and without the Cd shell is assumed to be attributable solely to the thermal neutron fluence. The results are presented in Table 2.3.1. The total fluence, the fluence above 0.414 eV, and the thermal fluence (i.e., < 0.414 eV) are represented by ϕ_T , ϕ_{Cd} , and ϕ_t respectively.

The redetermination of the responses of the TLD-600 elements to thermal neutrons is built upon the following premises (assuming scatter to be negligible):

- 1) the in-air response when the Cd-shell is on the sphere (A_{Cd}), is attributable to incident epi-Cd neutrons, those above 0.414 eV,
- 2) the in-air response when the Cd-shell is removed from the sphere (defined as A , which is not the same A of Eqns. 1.7.1, 1.7.3, and 1.7.4) is attributable to incident thermal and epi-Cd neutrons (to ϕ_t and ϕ_{Cd}),
- 3) the on-phantom response without the sphere's Cd-shell (Ph), is

Table 2.3.1 Fluence distribution for TLD-600 sensitivity irradiations using $^{252}\text{Cf}_{\text{D2O}}$ with and without the Cd shell.

Source configuration	Distributed fluence		
	ϕ_{T} (> 0.025 eV)	ϕ_{Cd} (> 0.414 eV)	ϕ_{t} (0.025 - 0.414 eV)
$^{252}\text{Cf}_{\text{D2O}(\text{Cd})}$ ^a		24.94	-
$^{252}\text{Cf}_{\text{D2O}(\text{no Cd})}$ ^a	28.17	24.94	3.24

^a Units = cm^{-2}

attributable to incident thermal (ϕ_{t}) and incident epi-Cd (ϕ_{Cd}) neutrons, plus albedo thermal and albedo epi-Cd neutrons,

- 4) the on-phantom response when the Cd-shell is on the sphere (Ph_{Cd}), is attributable to incident epi-Cd (ϕ_{Cd}) and albedo epi-Cd neutrons.

The first two assumptions are applied to calculate the TLD-600 sensitivity to incident thermal neutrons. Subtracting the in-air response with the Cd-shell, A_{Cd} , from the in-air response without the Cd shell, A , and dividing by the thermal fluence, ϕ_{t} , provides the sensitivity to incident thermal neutrons, i.e., $I_{\text{t}} = (A - A_{\text{Cd}}) / \phi_{\text{t}}$. The last two assumptions advocate determination of the total thermal neutron sensitivity by subtracting the on-phantom response with the Cd-shell, Ph_{Cd} , from the on-phantom response without the Cd shell, Ph , and dividing by the thermal fluence, i.e., $T_{\text{t}} = ((\text{Ph} - \text{Ph}_{\text{Cd}}) / \phi_{\text{t}})$. This provides the sensitivity to both incident and albedo thermal neutrons. The sensitivity to albedo thermal neutrons is determined by subtracting the incident thermal neutrons sensitivity, I_{t} , from the total thermal neutron sensitivity, T_{t} , i.e., $\text{Alb}_{\text{t}} = T_{\text{t}} - I_{\text{t}}$. The experimentally determined TLD-600 responses, in ^{137}Cs mR equivalent, are presented in Table 2.3.2, and the calculated sensitivities, in mR cm^{-2} , are presented in Table 2.3.3.

Table 2.3.2 TLD-600 response in ¹³⁷Cs mR equivalent.

Source configuration	²⁵² Cf _{D2O} (Cd)		²⁵² Cf _{D2O} (no Cd)	
	A _{Cd}	Ph _{Cd}	A	Ph
TLD-600 (Cd) ^a	192.04	1173.23	242.12	1417.76
TLD-600 (Plastic) ^a	242.12	1965.96	592.63	1359.96

^a Units = mR

Table 2.3.3 TLD-600 sensitivities in ¹³⁷Cs equivalent (10⁻⁵ mR cm²).

	I _t	Alb _t	T _t	I _{epi}	A _{epi}	T _{epi}
TLD-600 (Cd) ^a	1.55	6.0	7.55	0.77	3.93	4.70
TLD-600 (Plastic) ^a	10.80	7.88	18.68	0.97	4.48	5.55

2.4 REDEFINITION OF ENERGY INTERVALS (EI)

In principle the CPND operates much like the TDU. Four components (or detectors) with differing thresholds and response characteristics are utilized to determine the neutron spectral information. The rationale for subdividing energy range encountered in typical radiation protection environments, (of 0.025 eV to 15 MeV), into four segments or energy intervals (EI) is described. Each of the CPND components is then described in terms of its average sensitivity in each EI multiplied by the fluence in that EI.

Selection of EIs

During the process of redefining the four EIs, the refined R(E)s of the CPND's TLD-600 elements and the refined R(E)s of the BD-100R and BDS-1500 were considered. There were three primary factors involved in selecting the EIs: 1) the apparent natural break or drop in sensitivity of the BDS-1500 and BD-100R, 2) the Cd cutoff at 0.414 eV and 3) the points that correspond to the change in the

fluence-to-dose equivalent conversion factors as defined by the International Commission on Radiological Protection in Publication 21, i.e., ICRP 21 h₁ (ICRP 1973). The objective was to define the EIs so as to best optimize these criteria. The new EIs (thermal, slow, medium and fast) were redefined as follows:

- thermal = ≤ 0.414 eV,
- slow = 0.414 eV - 0.1 MeV,
- medium = 0.1 MeV - 1 MeV, and
- fast = 1 MeV - 15 MeV.

For comparison, Liu's EIs are given:

- thermal = ≤ 0.414 eV,
- slow = 0.414 eV - 0.15 MeV,
- medium = 0.15 MeV - 1.5 MeV, and
- fast = 1.5 MeV - 10 MeV.

For convenience, the fluence in each EI will be defined as the fast fluence (ϕ_f), medium fluence (ϕ_m), slow fluence (ϕ_s) and thermal fluence (ϕ_t), with the summation of these providing the total fluence (ϕ_T) for the spectrum.

The EI sensitivity (S_{EI}) of each component is taken to be the average sensitivity, in response per unit neutron, of that component, for that EI. Thus, the $R(E)$ of each component may be both visualized as a step function (Fig. 2.4.1) and represented numerically by the equation,

$$R_t = \sum_{EI = thermal}^{fast} (S_{EI} \times \phi_{EI}), \quad (2.4.1)$$

where

R_t = total response of the component,

S_{EI} = neutron sensitivity of the component for the EI, and

ϕ_{EI} = neutron fluence in the EI.

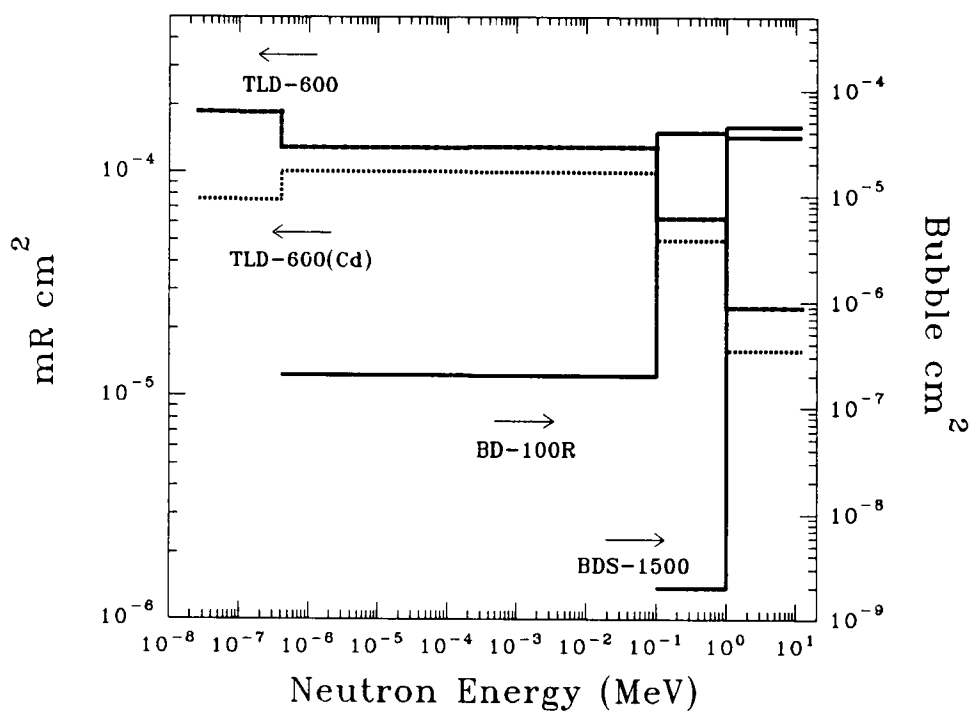


Fig. 2.4.1 Step function: average sensitivity in neutron response per unit fluence

Thus, the total response of the plastic covered TLD-600 is seen to be its S_f multiplied by ϕ_f , plus its S_m multiplied by ϕ_m , plus its S_s multiplied by ϕ_s , plus its S_t multiplied by ϕ_t . An analogous correspondence exists for the remaining three components. A comparison of Liu's EIs and sensitivities and the new EIs and sensitivities for each component are provided in Table 2.4.1 and Table 2.4.2.

2.5 MATRIX ALGORITHM AND SPECTRUM DECONVOLUTION

Deconvolution of the spectral results is grounded upon the assumption that the fluence in each EI is uniformly distributed over the EI, i.e., the fluence in the medium EI (0.1 - 1 MeV) is uniformly distributed between 0.1 and 1 MeV. This is assumed to be the case for each of the EIs, thermal, slow, medium and fast.

A comparison between the original stripping method and the new matrix algorithm for spectrometric deconvolution is presented.

Stripping Methodology

The original (Liu) methodology utilized simple stripping or subtraction to determine the fluences in each EI. An alternative methodology utilizing a four-by-four matrix, or four simultaneous equations, was developed as part of the modification.

Liu determined the ϕ_f from the BDS-1500 response, assuming the BDS-1500 responded only to neutrons above 1.5 MeV. The ϕ_m was then determined by subtracting the BDS-1500 response from the BD-100R assuming a BD-100R threshold of 150 keV.

Because TLD-600 is sensitive to photons and neutrons, it is necessary to isolate the neutron portion of the TLD-600 response. To accomplish this, a TLD-700 element with identical Cd or plastic covering is paired with each TLD-600 element. Each of the elements are calibrated to ^{137}Cs photons. Subtracting the paired TLD-700 response from the TLD-600 response corrects for the response to photons from both the radiation field and from the photons produced by the n- γ capture reaction of the Cd filter. Assuming that the TLD-700 response to neutrons is negligible and

Table 2.4.1 Original (Liu) CPND EIs, sensitivities and h_{ϕ} (EIs).

	Thermal 0.025-0.414 eV	Slow 0.414 eV-0.15 MeV	Medium 0.15-1.5 MeV	Fast 1.5-10 MeV
BDS-1500 ^a	-	-	-	5.0
BD-100R ^a	-	-	5.1	4.0
Total-Albedo ^b	18.4	-	-	-
Albedo ^b	14.7	5.6	3.8	1.6
Average h_{ϕ} (10^{-10} Sv cm ²)	h_t 0.11	h_s 0.45	h_m 2.66	h_f 4.05

^a Units = 10^{-5} bu cm²

^b Units = 10^{-5} mR cm²

Table 2.4.2 Modified (New) CPND EIs, sensitivities and h_{ϕ} (EIs).

	Thermal 0.025-0.414 eV	Slow 0.414 eV-0.1 MeV	Medium 0.1-1 MeV	Fast 1-15 MeV
BDS-1500 ^a	-	-	0.0002	4.5
BD-100R ^a	-	0.02	4.0	3.6
TLD-600(Cd) ^b	7.6	20	5.0	1.6
TLD-600 ^b	18.7	13	6.3	2.5
Average h_{ϕ} (10^{-10} Sv cm ²)	h_t 0.11	h_s 0.16	h_m 2.5	h_f 4.1

^a Units = 10^{-5} bu cm²

^b Units = 10^{-5} mR cm²

that the Cd cover absorbs the thermal neutrons on that element, it is presumed that the difference in response of the Cd-covered TLD-600 and the plastic-covered TLD-600 is simply attributable to the absorption of incident thermal neutrons by the Cd cover. Therefore, subtraction of the Cd-covered response from the plastic-covered response should provide a measure of the incident thermal fluence or ϕ_t . Next, ϕ_s was calculated by subtracting the determined ϕ_t , ϕ_m and ϕ_i from the plastic covered TLD-600 response.

In contrast, the seemingly absolute thresholds of 150 keV and 1.5 MeV for the BD-100R and BDS-1500 respectively were neither absolute, i.e., the response below which was assumed to be negligible, nor representative of the actual threshold in the laboratory. Note that the R(E)s of the BTI detectors were originally derived from the theoretical response calculated at 20°C. A more in-depth look at temperature related effects will be discussed in Section 4.3. For now let it suffice to state that the empirical measurements of the response to monoenergetic neutrons indicated that actual thresholds of 100 keV and 1 MeV were more accurate and that both detectors respond below these thresholds. This cannot be ignored without adversely effecting the spectral results obtained by the CPND (Section 2.2 and 2.4). Because the CPND can be described by four equations (one for each component) with four unknowns (the ϕ_{EIs}), it was felt that a method of deriving the spectral information by simultaneously solving these equations (thereby utilizing all the available information), would provide results which were more accurate. This was the reason for developing the matrix deconvolution algorithm.

Definition of matrix equations

Four equations relating the S_{EI} (Table 2.4.2) to the total response of the four components (expressed by Equation (2.4.1)) have been realized and are presented in Equations 2.5.1 - 2.5.4:

$$R_{TLD-600} = 18.7 \times 10^{-5} \times \phi_t + 13 \times 10^{-5} \times \phi_s + 6.3 \times 10^{-5} \times \phi_m + 2.5 \times 10^{-5} \times \phi_i \quad (2.5.1)$$

$$R_{TLD-600(Cd)} = 7.6 \times 10^{-5} \times \phi_t + 20 \times 10^{-5} \times \phi_s + 5 \times 10^{-5} \times \phi_m + 1.6 \times 10^{-5} \times \phi_i \quad (2.5.2)$$

$$R_{BD-100R} = 0x\phi_t + 2.0x10^{-7}x\phi_s + 4.0x10^{-5}x\phi_m + 3.6x10^{-5}x\phi_f \text{ and} \quad (2.5.3)$$

$$R_{BDS-1500} = 0x\phi_t + 0x\phi_s + 2.0x10^{-9}x\phi_m + 4.5x10^{-5}x\phi_f \quad (2.5.4)$$

These four equations with the four unknowns can be arranged in the form:

$$\begin{bmatrix} R_{TLD-600} \\ R_{TLD-600(Cd)} \\ R_{BD-100R} \\ R_{BDS-1500} \end{bmatrix} = \begin{bmatrix} 18.7x10^{-5} & 13x10^{-5} & 6.3x10^{-5} & 2.5x10^{-5} \\ 7.6x10^{-5} & 20x10^{-5} & 5x10^{-5} & 1.6x10^{-5} \\ 0 & 2.0x10^{-7} & 4.0x10^{-5} & 3.6x10^{-5} \\ 0 & 0 & 2.0x10^{-9} & 4.5x10^{-5} \end{bmatrix} \times \begin{bmatrix} \phi_t \\ \phi_s \\ \phi_m \\ \phi_f \end{bmatrix}$$

Matrix inversion

Taking the above four-by-four matrix, and inverting it, produces four new equations describing each ϕ_{EI} in terms of the response of each CPND component:

$$\phi_t = 7624.38 * R_{TLD-600} - 4716.3 * R_{TLD-600(Cd)} - 5546.13 * R_{BD-100R} + 2078.04 * R_{BDS-1500} \quad (2.5.5)$$

$$\phi_s = -2763.92 * R_{TLD-600} + 6800.7 * R_{TLD-600(Cd)} - 4147.82 * R_{BD-100R} + 2435.74 * R_{BDS-1500} \quad (2.5.6)$$

$$\phi_m = 13.82 * R_{TLD-600} - 34 * R_{TLD-600(Cd)} + 25021.74 * R_{BD-100R} - 20012.98 * R_{BDS-1500} \quad (2.5.7)$$

$$\phi_f = -0.0006 * R_{TLD-600} + 0.0015 * R_{TLD-600(Cd)} - 1.11 * R_{BD-100R} + 22223.11 * R_{BDS-1500} \quad (2.5.8)$$

After subtracting the gamma component from the TLD-600 response, applying a TCC (Equation 2.2.1) to the BD responses, which normalizes the data to a 1 bubble per 0.01 mSv ²³⁹PuBe calibrated detector (the reference point for the S_{EI} s and response functions) and after applying appropriate temperature corrections to compensate the BD response for irradiation temperatures greater than 20°C (by Eqn. 2.2.2), these normalized responses are then substituted into Equations 2.5.5 - 2.5.8 which are solved to provide the measured spectrum broken down into its constituent EI fluences, ϕ_f , ϕ_m , ϕ_s , and ϕ_t .

2.6 DOSE EQUIVALENT CONVERSION

The next step is to convert the EI fluences to dose equivalent. The dose equivalent produced by neutrons in each EI (H_{EI}) is calculated by multiplying the EI

fluences, $\phi_{f,m,s}$ & ν by their respective average h_ϕ ,

$$H_{EI} = \phi_{EI} \times \bar{h}_{\phi_{EI}}. \quad (2.6.1)$$

The average $h_\phi(EI)$ is defined as the average value of the h_ϕ over the EI. The average is obtained from a ln-ln interpolation of the ICRP 21 h_ϕ values. The calculated average $h_\phi(EI)$ s are listed in Table 2.4.2. The total neutron dose equivalent, H_T , is derived from the summation of the H_{EI} s contributed by each EI,

$$H_T = \sum_{EI=t}^f H_{EI} = H_t + H_s + H_m + H_f \quad (2.6.2)$$

In light of the volatile environment surrounding neutron dosimetry, i.e., the proposed increase in the neutron quality factor, reduction of the annual dose equivalent limits and the various dose equivalent reporting conventions employed, this simple spectrum affords a sure footing upon which to base the neutron dose equivalent. Because fluence is real and as such affords the luxury of applying various reporting conventions, as the situation dictates, a solid foundation is laid upon which to build a personnel neutron dosimetry system. We will now address the spectrometric and neutron dose equivalent performance of the modified CPND for the ten irradiation spectra.

Chapter III

PERFORMANCE EVALUATION AND ANALYSIS OF RESULTS

The performance of the modified CPND was assessed by comparison of the spectrometric (ϕ_{EI}) and dose equivalent results (H_{EI} and H_T) to reestablished reference dosimetry (necessitated by the new EIs) and the original results. A description of: 1) the field and source irradiations conditions, 2) the previous performance results of Liu, 3) the reassessment of the reference spectra and dosimetric values, and 4) performance reevaluation are provided.

3.1 INTRODUCTION

The performance of the CPND had previously been tested in five pure and mixed field radioisotopic neutron spectra and in five *in situ* neutron spectra at ORNL. The radioisotopic spectra were obtained from various combinations of $^{238}\text{PuBe}$, and ^{252}Cf moderated by polyethylene (PE) and D_2O . The average neutron energies of these sources are 4 MeV, 0.65 MeV (at 2m) and 0.55 MeV respectively. Five locations at ORNL's Transuranic Processing Plant (TRU) and the High Flux Isotope Reactor (HFIR), which were designed to provide quantities of transuranium and transcalifornium elements, were selected as sites for the *in situ* measurements.

During the *in situ* measurements a CPND was placed on the front and back of a 40 x 40 x 20 cm polymethyl methacrylate (PMMA) phantom to approximate a 4π measuring geometry. Whenever possible the direction of the radiation source was determined and the phantom was oriented with the front facing it. For the single-source and mixed-source irradiations, at least three CPNDs were placed on the front face of the phantom, and the results were averaged. A more in-depth description of the irradiation procedure is available in ORNL-6593, *The Development, Characterization and Performance Evaluation of a New Combination Type Personnel*

Dosimeter (Liu 1989).

Radioisotopic neutron sources

The radioisotopic irradiations were conducted using the neutron sources available at the Radiation Calibration Laboratory (RADCAL). The five spectra were $^{252}\text{Cf}(\text{PE})$, $^{238}\text{PuBe}$, $^{252}\text{Cf}(\text{D}_2\text{O})$, a combination of $^{238}\text{PuBe}$ and ^{252}Cf (MIX(2)) and a combination of $^{252}\text{Cf}(\text{PE})$, $^{252}\text{Cf}(\text{D}_2\text{O})$ and $^{238}\text{PuBe}$ (MIX(3)).

Working environments

The CPND was subjected to real-world work environments for which neutrons were present. The sites selected were the cave area, glove box, waste transfer area, control room and the analytical laboratory located at TRU and HFIR.

Reference Dosimetry

The reference spectra for the *in situ* and the ^{252}Cf moderated by polyethylene irradiations were determined from the unfolding of Bonner multi-sphere spectrometer (BMS) measurements provided by Dr. Ferenc Hajnal of the Environmental Measurements Laboratory (EML), New York (Liu 1989). During the original measurements two or more 100 second measurements were taken with each of the twelve detectors in the BMS set. The position of the BMS set was adjacent to the CPND location for each spectra. The reference spectra for the other radioisotopic irradiations were taken from emission spectra available in the open literature (for $^{238}\text{PuBe}$ [Block et al. 1967] and for $^{252}\text{Cf}(\text{D}_2\text{O})$ [IAEA 1985]). The original reference values, H_{EF} , for both the radioisotopic and the *in situ* irradiations are provided Tables 3.3.1 and 3.3.2.

3.2 PREVIOUS PERFORMANCE

The previous CPND results, (both dose equivalent and spectrometric for the *in situ* and the radioisotopic categories) are compared to the derived reference values of total neutron dose equivalent and spectrum accuracy. The individual and overall

dose equivalent performance is evaluated according to the conventionally accepted methodology currently utilized by the Department of Energy Laboratory Accreditation Program (DOELAP) as outlined in the *Department of Energy Standard For The Performance Testing of Personnel Dosimetry Systems, DOE/EH-0027*, (DOE 1986). The performance index,

$$P_i = \frac{[(\text{measured}) - (\text{reference})]}{(\text{reference})}, \quad (3.2.1)$$

was calculated for each individual measurement and the bias,

$$B = \frac{1}{n} \sum_{i=1}^n P_i \quad (3.2.2)$$

standard deviation,

$$S = \left[\frac{\sum_{i=1}^n (P_i - B)^2}{n-1} \right]^{1/2}, \quad (3.2.3)$$

and tolerance level (L),

$$|B| + S \leq L \quad (3.2.4)$$

were calculated for each category to assess the relative accuracy of the results. It should be noted that the DOELAP includes an error term (E) to account for the potential error in the reference dosimetry of the irradiation laboratory, i.e., $|B| + S - E \leq L$. For our purposes, E can be neglected. The P_i provides an indication of the accuracy for individual measurements. The standard deviation, in our analysis, may be considered as an indicator of the precision of the measurements

within the respective irradiation category, either radioisotopic or *in situ*. The bias may be viewed as an indication of the overall accuracy of the measurements within each category. The tolerance level takes into consideration the combination of overall accuracy and precision within each category. The optimum detector would have zeros for all four values, P_i , S, B, and L. As stated in DOE/EH-0027, a value of $L = 0.30$ is considered as passing, and therefore, acceptable.

Dose equivalent performance utilizing the Liu method

First considering the H_T performance of each irradiation within the two categories, as indicated by the P_i values, the original results were all within $\pm 30\%$ for the *in situ* category while only one lay outside of $\pm 30\%$ for the radioisotopic category, i.e., 34% high for the $^{252}\text{Cf}(\text{D}_2\text{O})$ measurement (Tables 3.2.1 and 3.2.2). Overall, when compared to the DOELAP acceptance criteria, i.e., $L \leq 0.30$, the total neutron dose equivalent as measured by the original CPND was well within the acceptable range for the *in situ* category, with an $L = 0.12$, yet, was just barely acceptable for the radioisotopic category, with an $L = 0.30$ (note the bottom line of Tables 3.2.1. and 3.2.2). The results, as indicated by the bias values, indicate an average overresponse of 13% in radioisotopic spectra and an average underresponse of 8% for the *in situ* spectra. The standard deviations suggest that the original CPND more accurately measured the dose equivalent for the *in situ* spectra than it did for the radioisotopic spectra. The B and S values were calculated for each measurement in the two categories. These results appear in Tables 3.2.3 and 3.2.4. Now let us turn to consider the spectrometric capabilities of the original method.

Spectrometric performance utilizing the Liu method

The original spectrometric abilities of the CPND were good. Analysis of the spectrometric B, S and L for each EI in the two categories is presented in Table 3.2.5. The original CPND tended to underestimate the ϕ_m and consequently underestimate H_m , while overestimating ϕ_s and ϕ_f , consequently overestimating H_s and

Table 3.2.1. The original (Liu) measured dose equivalent (H_m and H_T) and calculated P_i results from the radioisotopic source measurements (CPND units = 0.01 mSv (1 mrem)).

	<u>$^{252}\text{Cf(PE)}$</u>		<u>$^{238}\text{PuBe}$</u>		<u>$^{252}\text{Cf(D,0)}$</u>		<u>MIX(2)</u>		<u>MIX(3)</u>	
	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i
H_t	3.15	-0.28	4.69	-	3.07	-	0.93	-	2.55	0.15
H_s	5.55	0.68	0.00	-	138.40	2.79	22.93	3.53	30.26	3.14
H_m	26.40	-0.13	6.58	-0.39	32.93	-0.49	10.67	-0.20	64.43	-0.29
H_f	41.10	-0.15	59.78	0.13	154.67	0.07	40.00	-0.05	402.05	0.10
H_T	76.20	-0.12	71.05	0.12	329.07	0.34	74.53	0.23	499.29	0.07

Standard Deviation = 0.17

Bias = 0.13

L = 0.30

Table 3.2.2. The original (Liu) measured dose equivalent (H_m and H_T) and calculated P_i results from the *in situ* measurements at TRU (CPND units = 0.01 mSv (1 mrem)).

	<u>GLOVE</u>		<u>CAVE</u>		<u>CNTRL</u>		<u>WASTE</u>		<u>LAB</u>	
	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i
H_t	17.38	-0.30	10.39	-0.12	0.03	-0.92	4.56	0.05	3.57	0.72
H_s	126.79	1.47	27.89	0.66	0.25	-0.77	60.85	1.64	72.54	2.39
H_m	169.69	-0.52	54.69	-0.29	3.21	-0.23	164.77	-0.18	131.70	-0.40
H_f	367.07	0.04	59.79	-0.07	4.95	0.45	174.12	-0.15	254.49	0.11
H_T	680.93	-0.13	152.76	-0.10	8.44	-0.07	404.30	-0.07	462.30	-0.02

Standard Deviation = 0.04

Bias = -0.08

L = 0.12

Table 3.2.3. The individual bias and standard deviation of the original CPND for the radioisotopic measurements.

	²⁵² Cf(PE)	²³⁸ PuBe	²⁵² Cf(D ₂ O)	MIX(2)	MIX(3)
B	0.03	1.11	1.36	1.05	0.78
S	0.44	2.39	1.83	1.73	1.59

Table 3.2.4. The individual bias and standard deviation of the original CPND for the *in situ* measurements.

	GLOVE	CAVE	CNTRL	WASTE	LAB
B	0.17	0.05	-0.37	0.34	0.70
S	0.89	0.42	0.62	0.87	1.21

Table 3.2.5. The EI bias, standard deviation and L value of the original CPND for the radioisotopic and *in situ* categories.

	Radioisotopic			<i>In situ</i>		
	B	S	L	B	S	L
H _t	1.71	2.10	3.82	-0.11	0.59	0.70
H _s	2.03	1.58	3.61	1.08	1.20	2.28
H _m	-0.30	0.14	0.44	-0.32	0.14	0.46
H _f	0.02	0.12	0.14	0.08	0.23	0.31
H _T	0.13	0.17	0.30	-0.08	0.04	0.12

H_T as evidenced by the values of B in Table 3.2.5. Thus, in some cases the "goodness" of the measured H_T could be conceived as a fortuitous combination of errors (note Tables 3.2.1 and 3.2.2).

From a cursory examination, one would conclude that the CPND measured the reference neutron spectrum with reasonable accuracy. The poorest performance was found when measuring spectra with large fluence components between 100 keV and 2 MeV and large thermal components. The consistent underestimation of H_s and H_f and the overestimation of H_m is felt to be attributable to the thresholds assumed for the BD-100R and BDS-1500. The overestimation of the ϕ_t for the $^{252}\text{Cf}(\text{D}_2\text{O})$ and $^{238}\text{PuBe}$ and the overestimation of H_s by greater than a factor of two for four of the ten spectra is believed to stem from two other weaknesses. These are: 1) the thermal neutron sensitivity assumed for the TLD-600 elements, and 2) accepting the subtraction of TLD-600(Cd) from TLD-600(plastic) as an accurate measure of ϕ_t . Let us now turn to consider the reassessment of the reference dosimetry and the results of the modified approach.

3.3 REASSESSMENT OF REFERENCE SPECTRA AND DOSIMETRIC VALUES

Because new EIs were defined for the CPND, it was necessary to recalculate the reference values for the ϕ_{EI} and H_{EI} for each of the test spectra. The original 26-energy group BMS data provided by EML and the reference spectra published in the open literature were used as the starting point. These spectral data were entered into a spreadsheet. Computations based on ln-ln interpolation were performed to determine the relative abundance of the neutrons and the spectra were broken down into 20 keV intervals from 0.025 eV to 15 MeV for each spectra using,

$$\ln(\phi_{E_m}) = \ln(\phi_{E_{upper}}) + \left[\left(\frac{\ln(E_u) - \ln(E_m)}{\ln(E_m) - \ln(E_{lower})} \right) \times ((\ln(\phi_{E_{lower}}) - \ln(\phi_{E_{upper}}))) \right], \quad (3.3.1)$$

then,

$$\phi_{E_m} = e^{\ln(\phi_{E_m})}, \quad (3.3.2)$$

where

$\phi_{E_m, \text{ upper and lower}}$ = the fluence at the m, upper and lower energies respectively.

The fluence in each EI was taken to be the sum of the 20 keV fluences within the EI. The dose equivalent for the 20 keV intervals ($H_{20 \text{ keV}}$) was calculated by multiplying each $\phi_{20 \text{ keV}}$ by the average h_ϕ for that 20 keV interval determined by a ln-ln interpolation of ICRP 21 h_ϕ . The H_{EI} was taken to be the summation of the $H_{20 \text{ keV}}$ within the EI, and the total H_T was taken to be the summation of all $H_{20 \text{ keV}}$ from 0.025 eV - 15 MeV. The observed difference in reference values between this work and the original stem from the different EIs. Liu's ϕ_m included the neutrons between 1 - 1.5 MeV, while these neutrons were included in the ϕ_f according to the modified EIs. Consequently, the reference H_f for the modified EIs would typically be greater than that of the original. It is believed that this approach is more consistent with the change in the ICRP 21 h_ϕ which occurs at about 1 MeV. Details of the "New" and Liu reference values of H_{EI} and H_T for both the radioisotopic and the *in situ* irradiations are provided in Tables 3.3.1. and 3.3.2.

3.4 PERFORMANCE REEVALUATION

The ϕ_{EI} , H_{EI} and H_T results from the radioisotopic and *in situ* irradiations were compared to reference values and the CPND performance prior to modifications. The performance index values of P, B, S and L were as calculated for the modified results as described in section 3.2. The modifications brought about improvements in the accuracy of the spectrometric and the total neutron dose equivalent results.

Dose equivalent performance

The dosimetric performance of the CPND is displayed in Tables 3.4.1 and 3.4.2. The ratio of the measured to new reference values are graphically depicted in Figures 3.4.1 and 3.4.2. T, S, M and F correspond to H_v , H_s , H_m , and H_f . The H_T L

Table 3.3.1. Comparison of original (Liu) and modified (New) reference values for radioisotopic neutron H_{EI} and H_{T} results (units = 0.01 mSv (mrem)).

	<u>$^{252}\text{Cf(PE)}$</u>		<u>$^{238}\text{PuBe}$</u>		<u>$^{252}\text{Cf(D}_7\text{O)}$</u>		<u>MIX (2)</u>		<u>MIX (3)</u>	
	NEW	LIU	NEW	LIU	NEW	LIU	NEW	LIU	NEW	LIU
H_{T}	56.70	48.45	55.21	52.67	147.68	145.20	48.99	42.10	432.97	365.84
H_{m}	19.06	30.30	7.62	10.80	63.99	64.40	13.49	13.33	85.76	90.78
H_{s}	3.40	3.30	0	0	34.66	36.53	5.62	5.06	21.69	7.37
H_{t}	4.29	4.35	0	0	0	0	0	0	2.15	2.21
H_{T}	83.47	86.40	62.83	63.46	246.13	246.13	60.49	68.1	542.57	466.14

Table 3.3.2. Comparison of original (Liu) and modified (New) reference values for neutron H_{EI} and H_{T} *in situ* measurements (units = 0.01 mSv (mrem)).

	<u>GLOVE</u>		<u>CAVE</u>		<u>CNTRL</u>		<u>WASTE</u>		<u>LAB</u>	
	NEW	LIU	NEW	LIU	NEW	LIU	NEW	LIU	NEW	LIU
H_{T}	450.62	352.95	79.7	64.35	6.52	3.42	250.23	205.11	278.71	228.62
H_{m}	246.14	352.95	56.76	76.57	3.16	4.18	137.74	200.55	148.67	220.60
H_{s}	38.87	51.31	12.89	16.77	0.86	1.11	17.44	23.02	14.12	21.41
H_{t}	23.97	24.71	11.57	11.85	0.33	0.36	4.21	4.33	2.13	2.08
H_{T}	759.6	781.92	160.92	169.54	11.66	9.07	409.62	433.01	443.64	472.71

* Units = 0.01 mSv (mrem)

Table 3.4.1. The modified CPND measured dose equivalent (H_{gr} and H_T) and the calculated P_i results for the radioisotopic measurements (CPND units = 0.01 mSv (1 mrem)).

	<u>$^{252}\text{Cf(PE)}$</u>		<u>$^{238}\text{PuBe}$</u>		<u>$^{252}\text{Cf(D,0)}$</u>		<u>MIX(2)</u>		<u>MIX(3)</u>	
	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i
H_i	4.56	0.06	0.09	-	0.00	-	0.29	-	2.14	0.00
H_j	2.40	-0.29	0.19	-	35.66	0.03	6.82	0.21	8.85	-0.59
H_m	31.77	0.67	6.76	-0.11	37.15	-0.42	11.79	-0.13	77.37	-0.10
H_r	46.30	-0.18	56.47	0.02	174.42	0.18	50.68	0.03	453.31	0.05
H_T	85.03	0.02	63.51	0.01	247.23	0.00	69.58	0.02	541.67	0.00

Standard Deviation = 0.01

Bias = 0.01

L = 0.02

Table 3.4.2. The modified CPND measured dose equivalent (H_{gr} and H_T) and the calculated P_i for the *in situ* measurements at TRU (CPND units = 0.01 mSv (1 mrem)).

	<u>GLOVE</u>		<u>CAVE</u>		<u>CNTRL</u>		<u>WASTE</u>		<u>LAB</u>	
	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i	CPND	P_i
H_i	20.34	-0.15	15.11	0.31	0.33	-0.06	3.16	-0.25	1.25	-0.41
H_j	37.32	-0.04	10.57	-0.18	0.71	-0.17	16.02	-0.08	19.25	0.36
H_m	202.98	-0.18	65.46	0.15	4.53	-0.43	184.64	0.34	143.25	-0.04
H_r	413.67	-0.08	67.30	-0.16	6.09	-0.07	182.63	-0.27	260.67	-0.06
H_T	674.31	-0.11	158.44	-0.02	11.66	0.07	386.45	-0.06	424.42	-0.04

Standard Deviation = -0.03

Bias = 0.07

L = 0.10

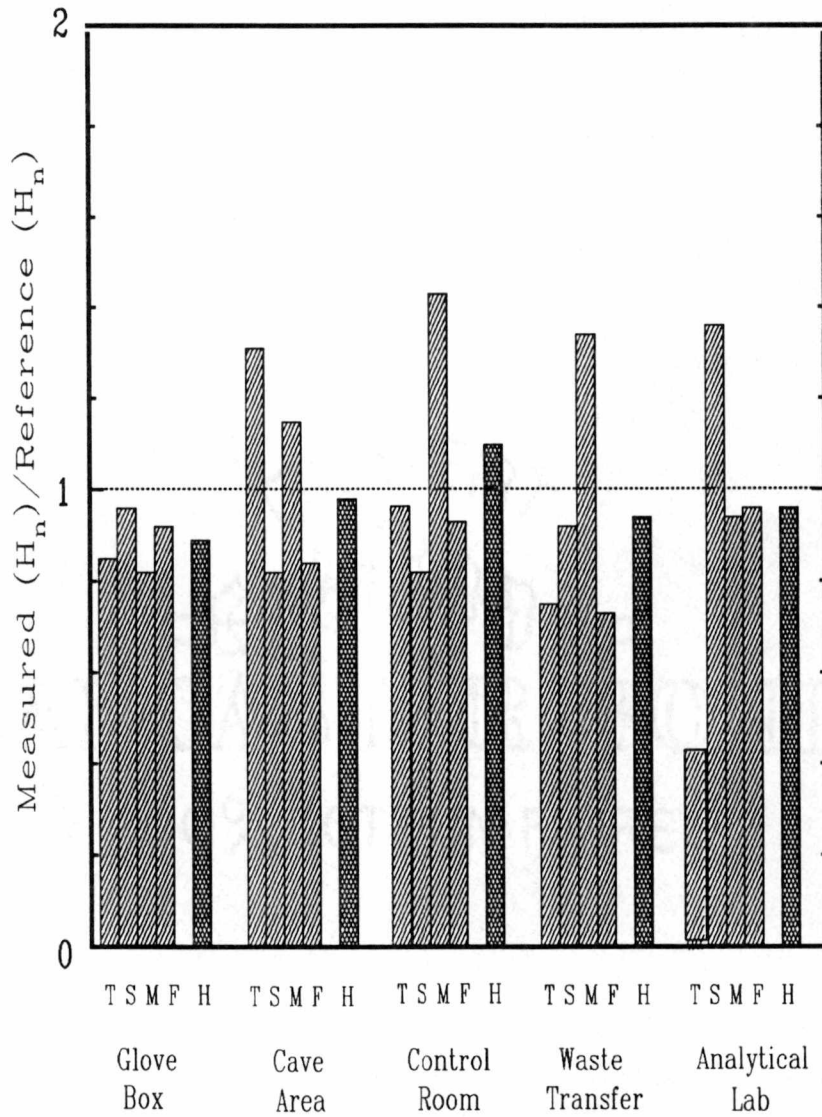


Fig. 3.4.1. The relative accuracy of the CPND to measure neutron dose equivalent (H_{EI} and H_T) for ORNL *in situ* spectra at TRU.

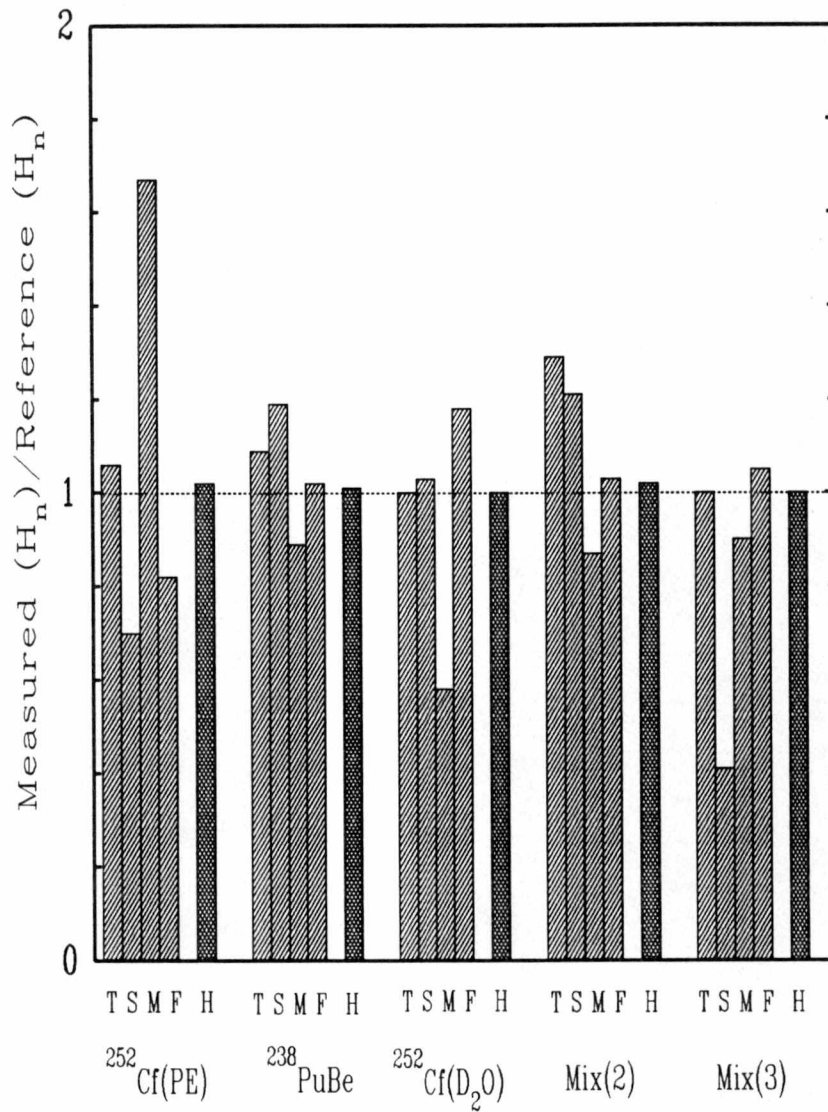


Fig. 3.4.2. The relative accuracy of the CPND to measure neutron dose equivalent (H_{EI} and H_T) of RADCAL source spectra.

value 0.02 and 0.10 for the radioisotopic and *in situ* categories respectively were well below the 0.30 limit of DOELAP. The P_i values of the individual H_T reveal that the worst performance for the radioisotopic measurements was 0.02 while the worst for the *in situ* measurements was -0.11. The B values, indicate an average overresponse of 1% in radioisotopic spectra and an average underresponse of 3% for the *in situ* spectra. The standard deviations suggest that the original CPND more accurately measured the dose equivalent for the *in situ* spectra than it did for the radioisotopic spectra, but only by 6%. Both were within 7%. The B and S values were calculated for each of the measurements in the two categories. These results appear in Tables 3.4.3 and 3.4.4. Now let us turn to consider the spectrometric capabilities of the original method.

Spectrometric performance

The spectrometric results of the modified CPND for both the radioisotopic and *in situ* spectra are presented in Figures 3.2.3 through 3.2.12 respectively. The reference values represented were derived from BMS measurements for the *in situ* and $^{252}\text{Cf}(\text{PE})$ values and from the published literature for the source spectra as described in Section 3.3. With the exception of $^{252}\text{Cf}(\text{PE})$, all other reference spectra for the radioisotopic irradiations are for the emission spectra only and, therefore, do not include the scatter component which would have been measured by the CPND. The overall B, S and L values were calculated for the H_{EIS} and H_{TS} in each category. These appear in Table 3.4.5.

3.5 ANALYSIS OF RESULTS

The modified CPND outperformed the original in overall dose equivalent results across the board (Table 3.5.1). It demonstrated improved accuracy and precision as evidenced by the improved B and S values. The modified CPND displayed improved H_n accuracy for eight of the ten spectra. For the other two, the original performance was better by 2% in the analytical laboratory and the same for

Table 3.4.3. The individual bias and standard deviation of the modified CPND for the radioisotopic measurements.

	$^{252}\text{Cf(PE)}$	$^{238}\text{PuBe}$	$^{252}\text{Cf(D}_2\text{O)}$	MIX(2)	MIX(3)
B	0.06	0.05	-0.05	0.10	-0.16
S	0.42	0.13	0.26	0.19	0.29

Table 3.4.4. The individual bias and standard deviation of the modified CPND for the *in situ* measurements.

	GLOVE	CAVE	CNTRL	WASTE	LAB
B	-0.11	0.03	0.03	-0.06	-0.04
S	0.06	0.24	0.27	0.28	0.32

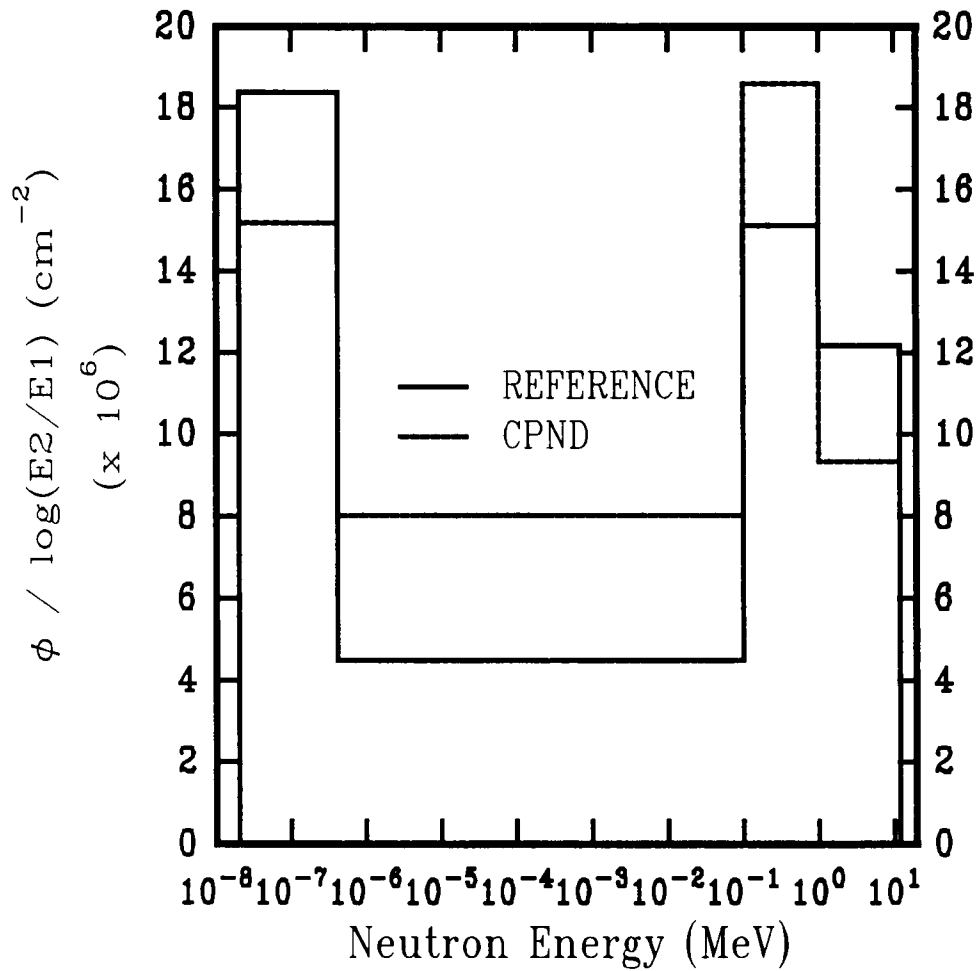


Fig. 3.4.3. Comparison of reference (BMS) and CPND measured spectra for the glove box at TRU.

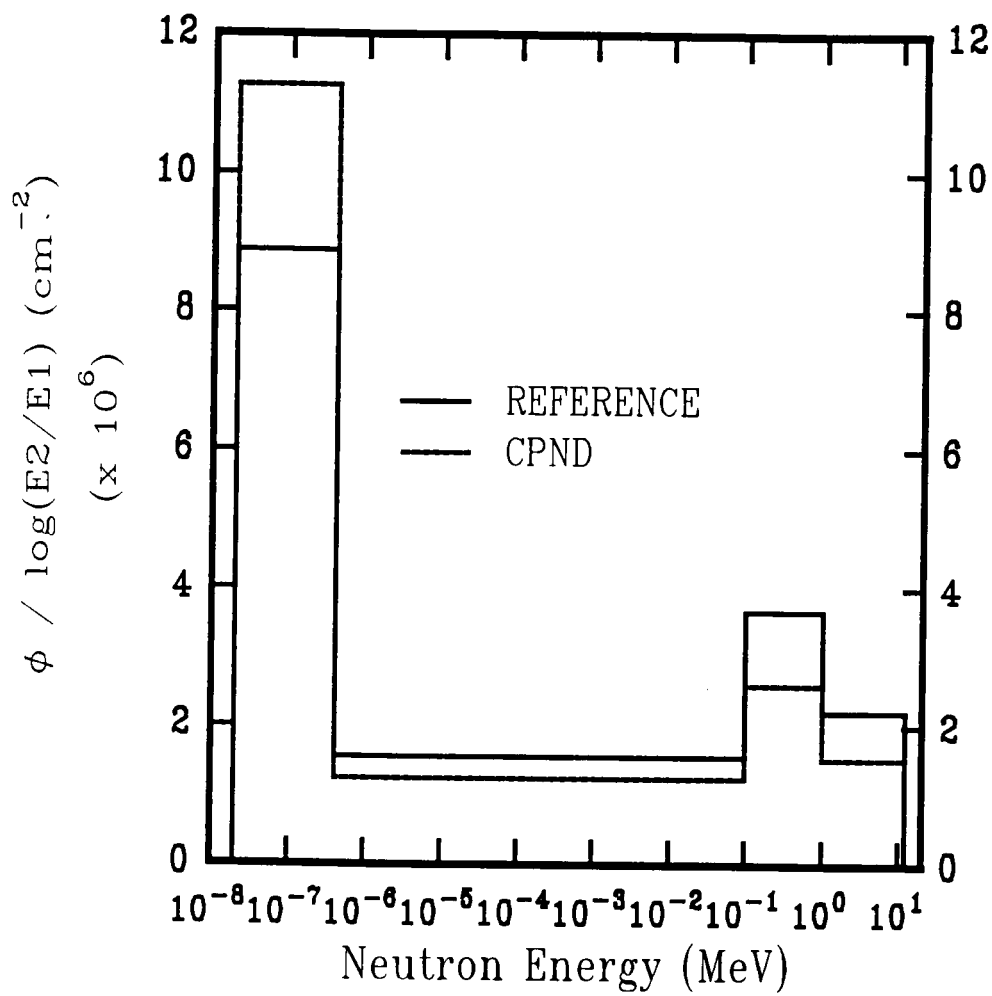


Fig. 3.4.4. Comparison of reference (BMS) and CPND measured spectra for the cave area at TRU.

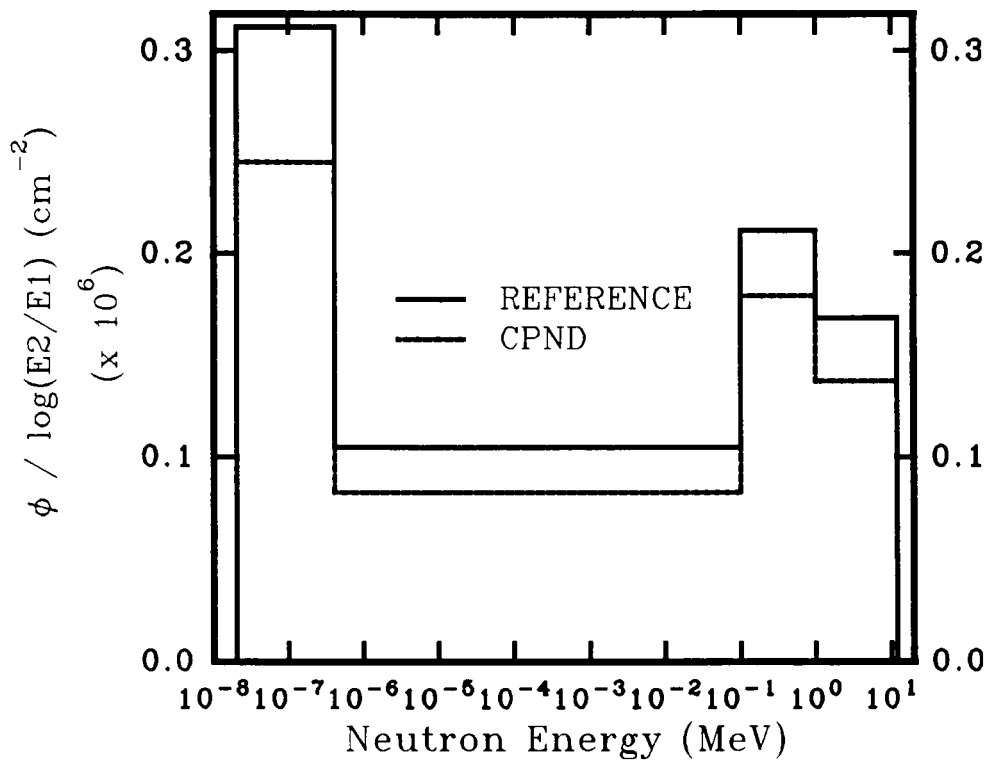


Fig. 3.4.5. Comparison of reference (BMS) and CPND measured spectra for the control room at TRU.

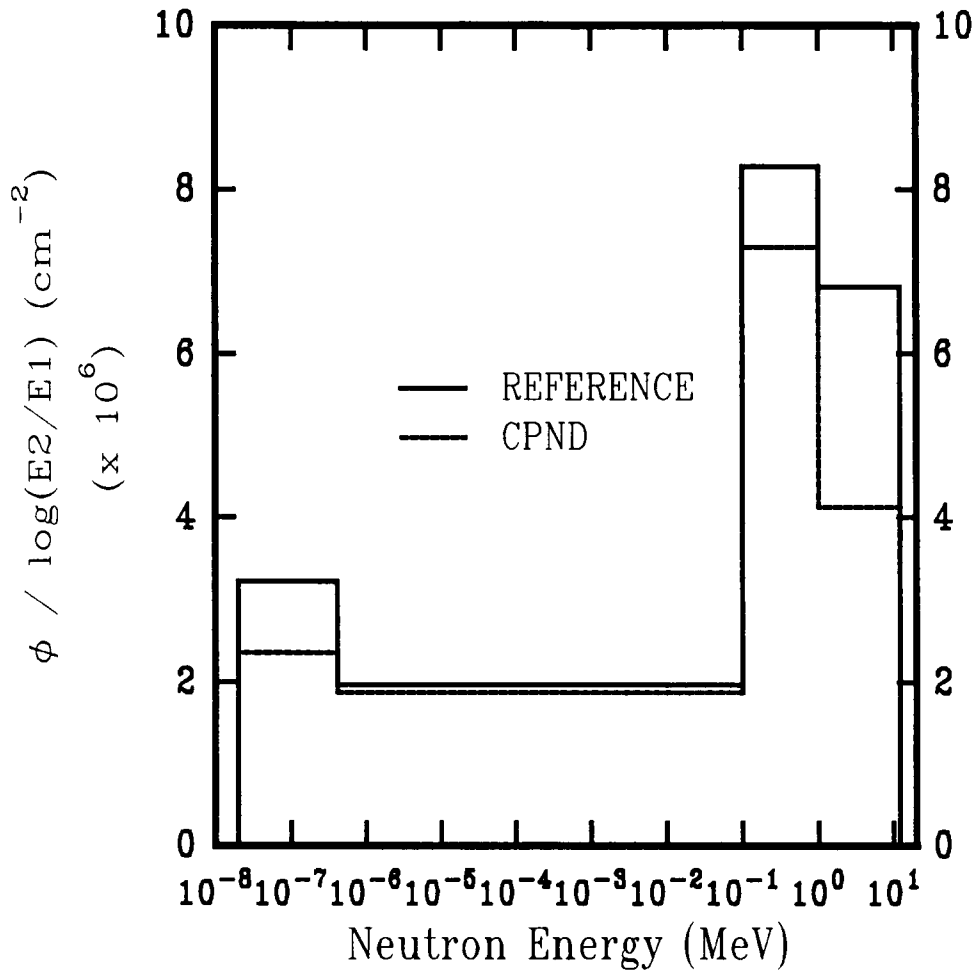


Fig. 3.4.6. Comparison of reference (BMS) and CPND measured spectra for the waste transfer area at TRU.

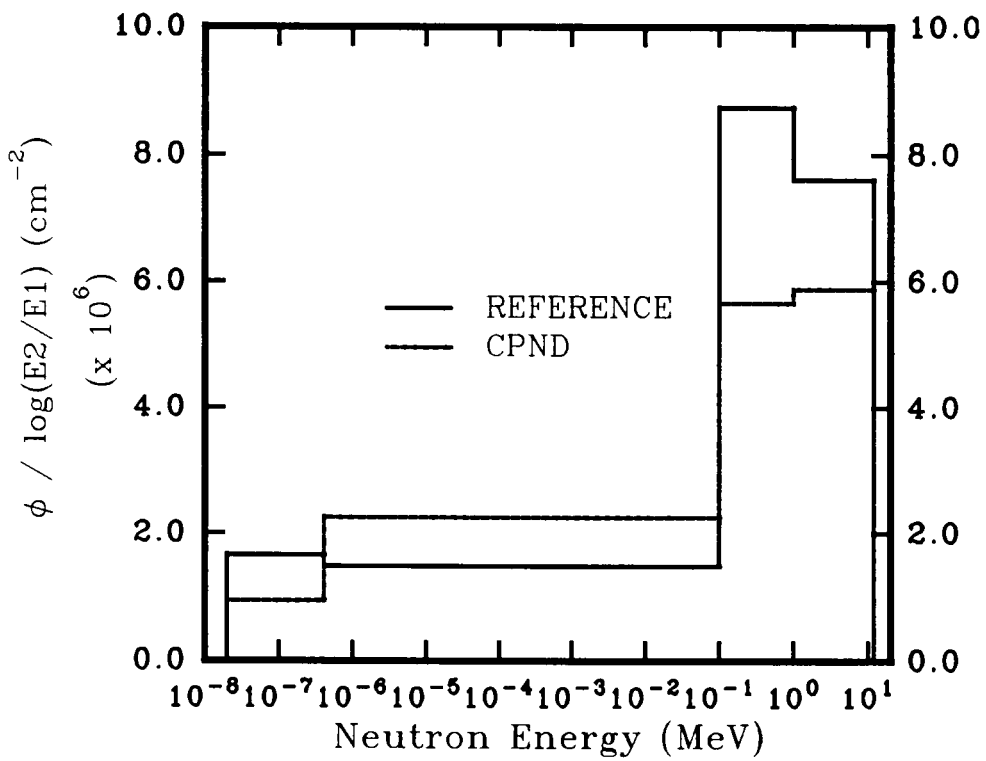


Fig. 3.4.7. Comparison of reference (BMS) and CPND measured spectra for the analytical lab at TRU.

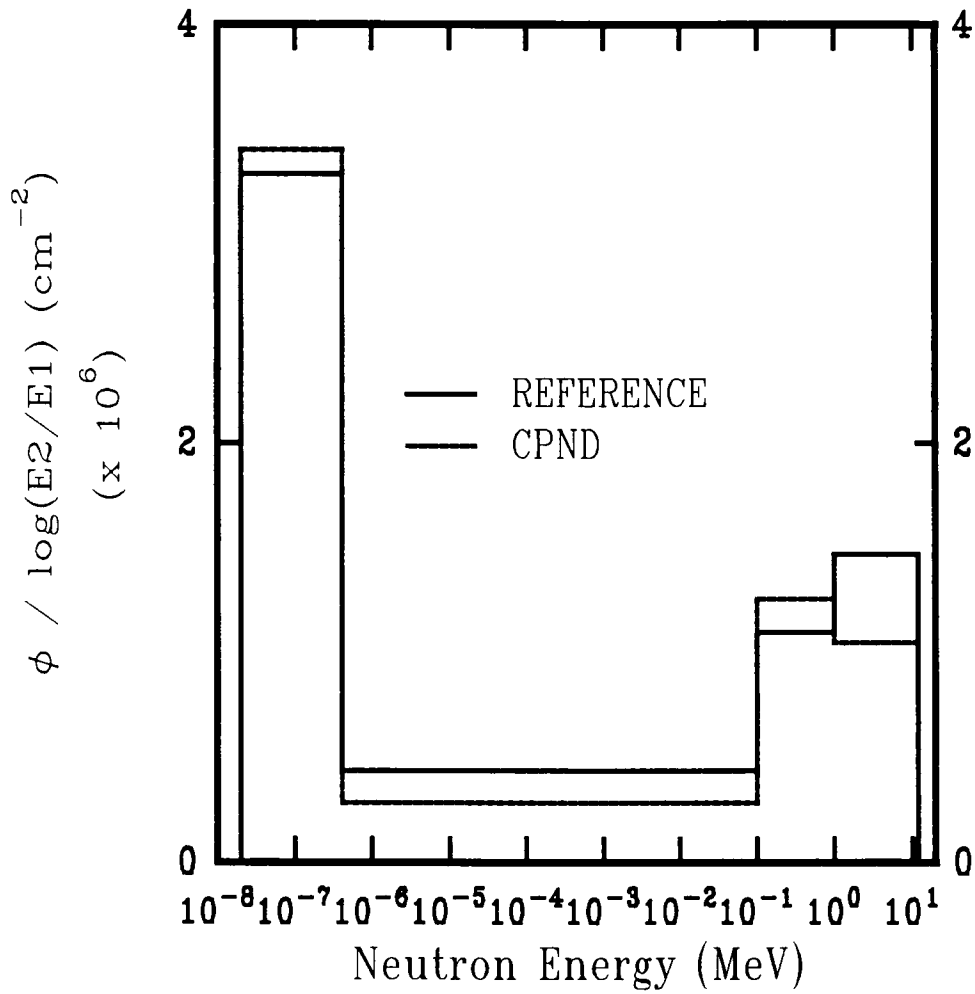


Fig. 3.4.8. Comparison of reference (BMS) and CPND measured spectrum for the $^{252}\text{Cf}(\text{PE})$ source at RADCAL.

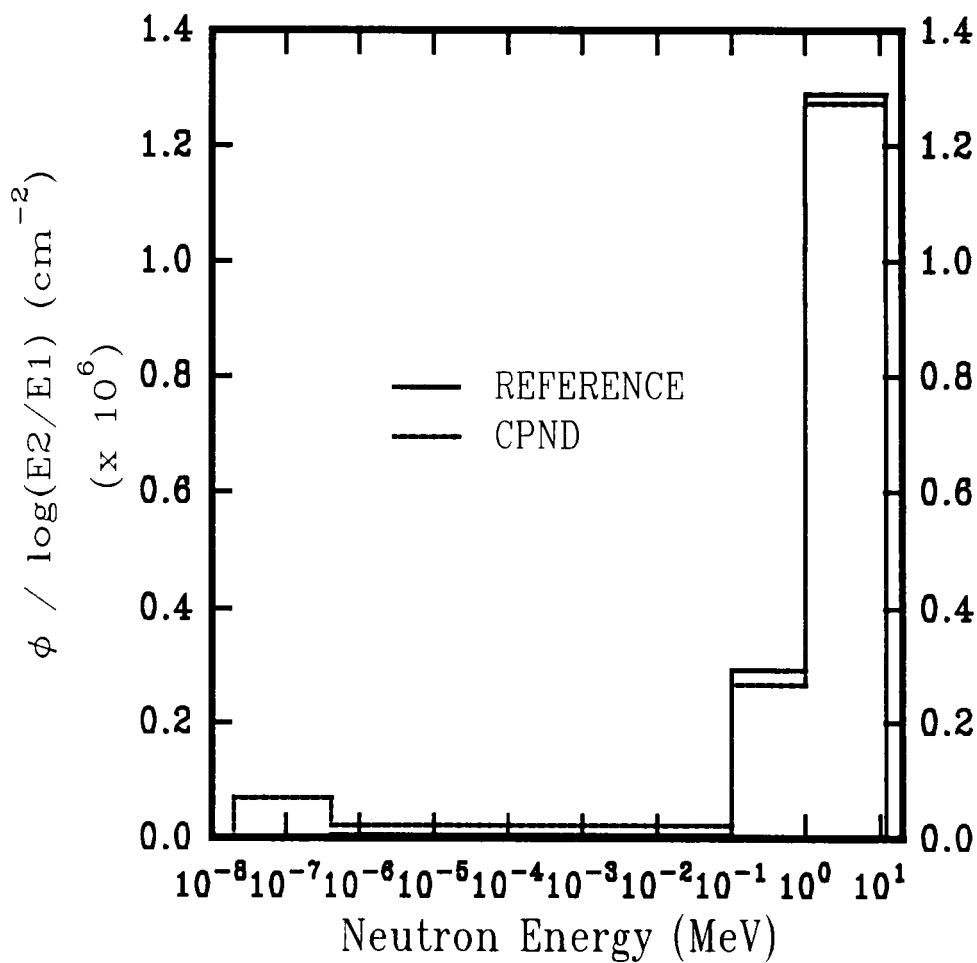


Fig. 3.4.9. Comparison of reference and CPND measured spectrum for the $^{238}\text{PuBe}$ source at RADCAL.

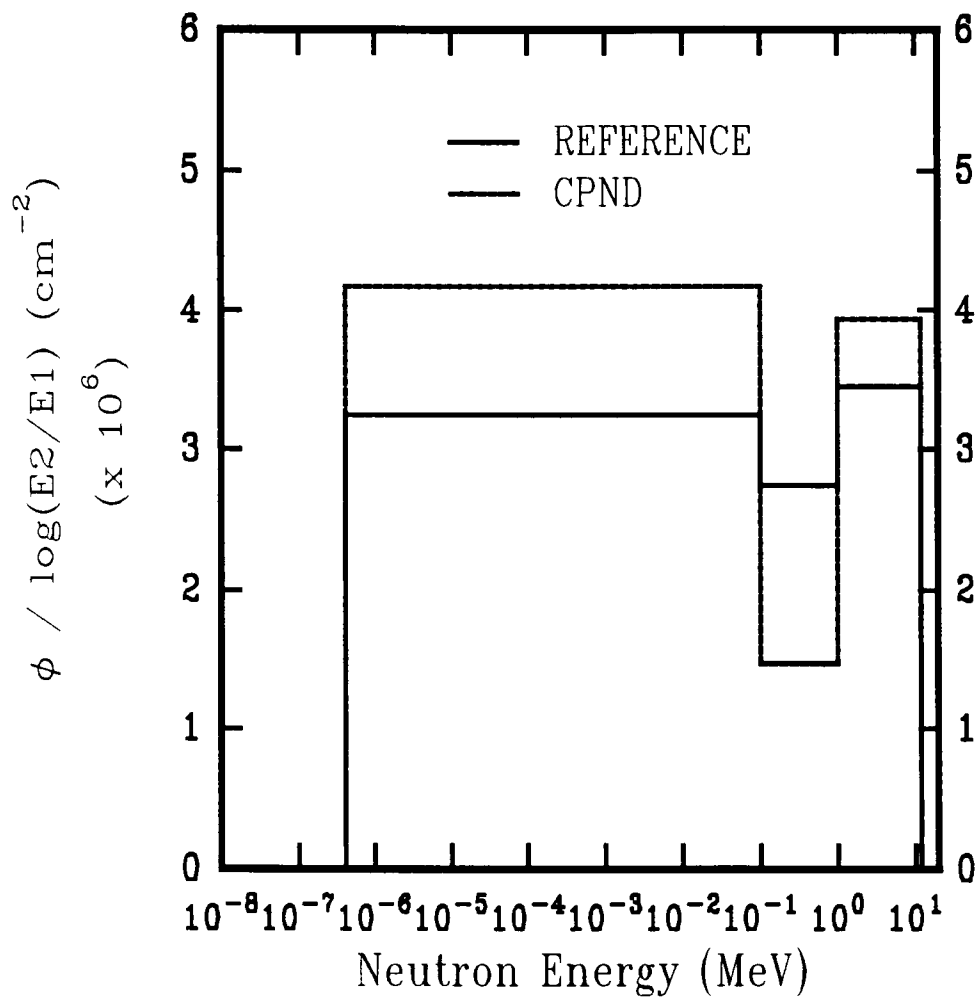


Fig. 3.4.10. Comparison of reference and CPND measured spectrum for the $^{252}\text{Cf}(\text{D}_2\text{O})$ source at RADCAL.

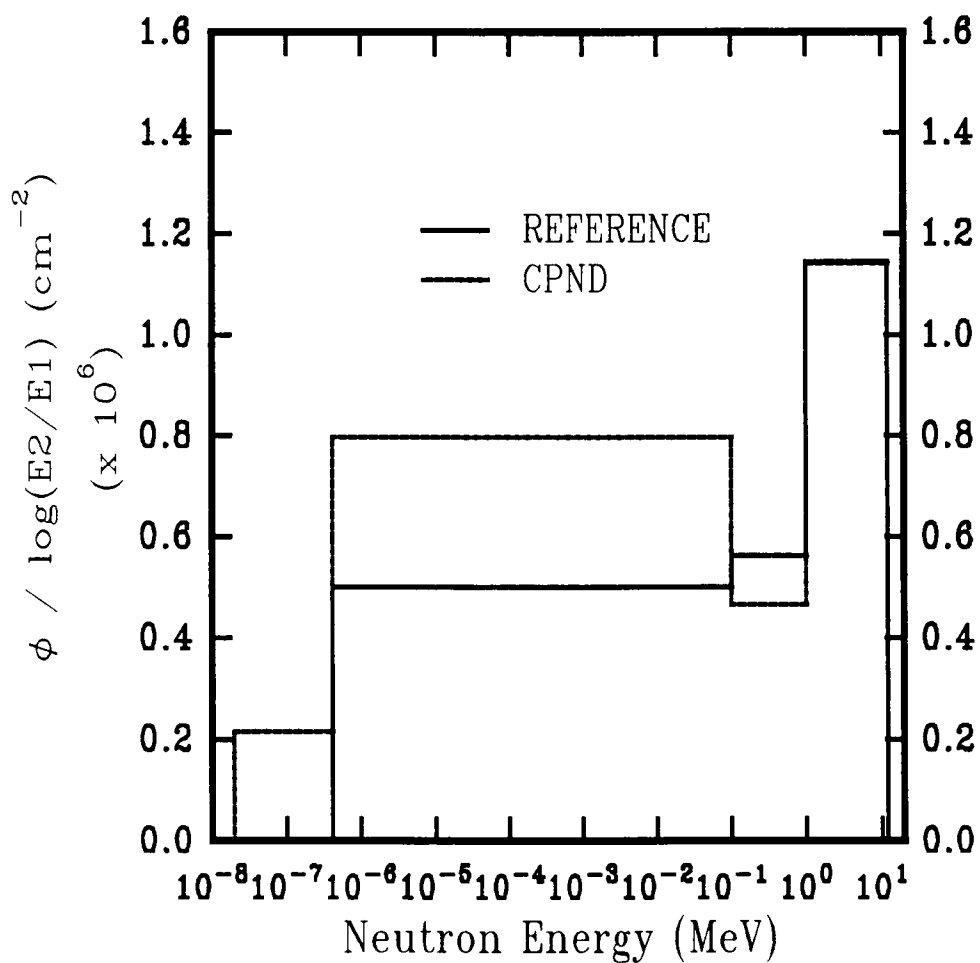


Fig. 3.4.11. Comparison of reference and CPND measured spectrum for a mixture of two RADCAL sources: $^{252}\text{Cf}(\text{D}_2\text{O})$ and $^{238}\text{PuBe}$.

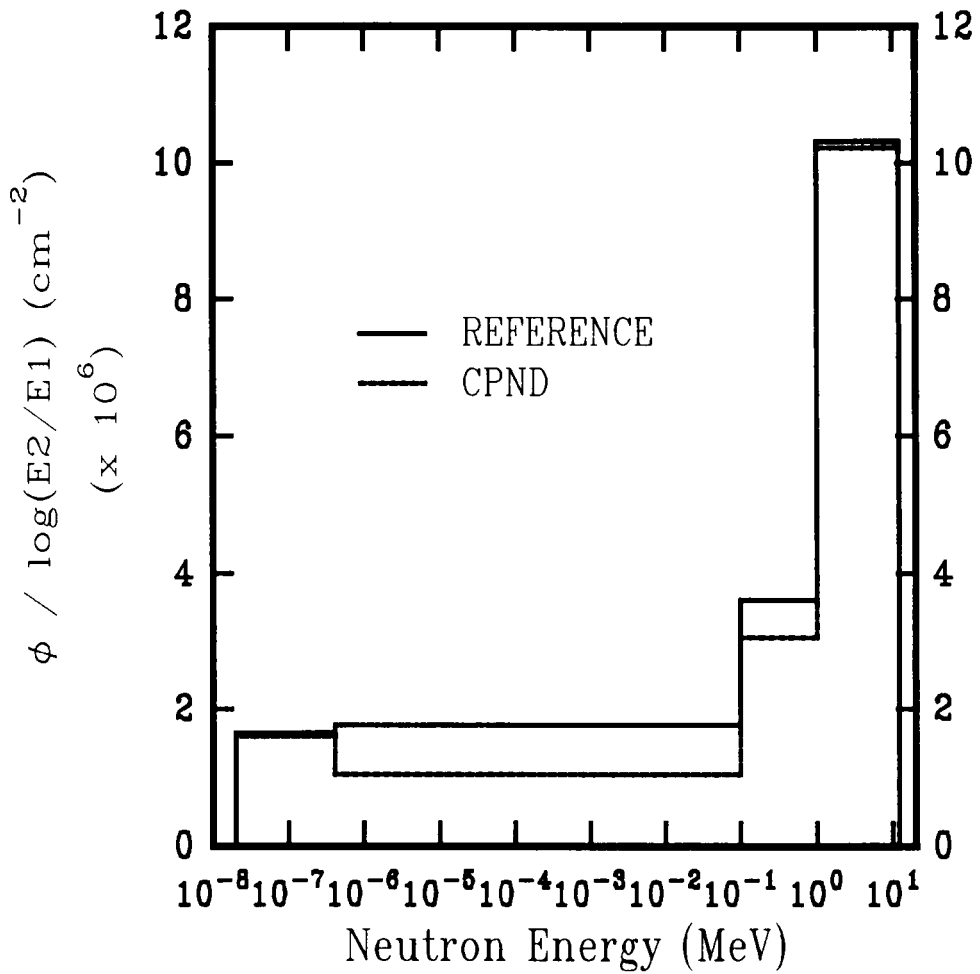


Fig. 3.4.12. Comparison of reference and CPND measured spectrum for mixture of RADCAL sources: $^{252}\text{Cf}(\text{D}_2\text{O})$, $^{252}\text{Cf}(\text{PE})$ and $^{238}\text{PuBe}$ (MIX(3)).

Table 3.4.5. The overall bias, standard deviation and L value of the modified CPND for the radioisotopic and *in situ* categories.

	Radioisotopic			<i>In situ</i>		
	B	S	L	B	S	L
H _i	0.09	0.12	0.21	-0.11	0.27	0.38
H _s	-0.09	0.35	0.44	-0.02	0.22	0.25
H _m	-0.02	0.40	0.42	1.14	0.25	0.40
H _f	0.02	0.13	0.15	-0.13	0.09	0.22
H _T	0.01	0.01	0.02	-0.03	0.07	0.10

Table 3.5.1 Comparison of the original and the modified overall performance indicators.

	Radioisotopic			<i>In situ</i>		
	B	S	L	B	S	L
Original	0.13	0.17	0.30	0.08	0.04	0.12
Modified	0.01	0.01	0.02	0.07	0.03	0.10

the control room. Overall a net improvement in H_T of 28% was achieved for the radioisotopic category and only 2% for the *in situ* category.

These results reveal that enhanced spectral resolution was obtained which produced an overall improvement in the dosimetric accuracy. The L value calculated for each EI reveals an improvement in spectrometric performance for all EI in both categories except for the fast in the radioisotopic category where the original performance was better by 1%. We therefore, conclude that the modified CPND demonstrated spectrometric and dose equivalent superiority over the original.

We will now take up a more philosophical venue as we survey some current assumptions about bubble detectors (such as useable lifetime, reproducibility, temperature affects and compensation methods, and theory of operation) and in turn, offer some alternative explanations. We will also offer an explanation of bubble growth, bubble memory and incompressible bubbles.

Chapter IV

SOME CURRENT ASSUMPTIONS AND ALTERNATIVE EXPLANATIONS

Investigative research and data analysis often unearth observations that are initially very curious and sometimes difficult, if not impossible, to explain by current paradigms. For the bubble detector, some of the more elusive items to explain have been:

- 1) useable lifetime,
- 2) variations in the reproducible response of a detector observed by different investigators and sometimes even the same investigator,
- 3) temperature affects and compensation methods,
- 4) bubble formation, growth and memory,
- 5) incompressible bubbles, and
- 6) a theory accurately predicting bubble nucleation.

In reply, some theories are presented that attempt to explain some of these more "mysterious" phenomena and question some of the methodologies employed to either compensate, control or explain them.

4.1 USEABLE LIFETIME

Studies have been conducted at the Naval Surface Warfare Center (NSWC) and ORNL with the goal of addressing the usable lifetime of the bubble detector. We will use this term loosely because of the complexity surrounding the issue. BTI claims a life span on the order of months before a noticeable decrease in sensitivity is encountered (Roy 1991). This life span presupposes a life style of moderation, i.e., recompression on a routine basis either daily or every other day. This is to minimize damage to the PAG caused by bubble growth (see Section 4.4). There seems to be

a correlation between an appreciable decrease in sensitivity and the time from initial sensitization to recompression. This may be associated with diffusion of the SHL into the surrounding medium which effectually reduces the number of potential nucleation sites, ergo a reduction in sensitivity.

The preliminary results from the NSWC studies should be considered inconclusive because of the testing conditions. For the majority of the failing detectors, the time between initial sensitization and recompression exceeded the weekly cycle suggested by BTI: " a period of up to a week between recompression cycles is possible without noticeable sensitivity changes or incompressible bubbles" (Roy 1991). NSWC was hoping to find a means of extending the time between recompressions to accommodate an exchange cycle of at least a month. According to BTI it is possible to manufacture bubble detectors that will remain sensitive for this period of time, but there is a trade-off. The expense is loss of reusability due to accumulation of incompressible bubbles (Roy 1991).

4.2 RESPONSE VARIATION

Several of the bubble detector researchers have observed unexplainable variations in their results. These variations were characterized by larger than desired standard deviations and variances observed in repeated irradiations of a single detector and during testing of the same detector type. It is our belief that unless the bubbles in a detector are allowed to grow excessively (the effects of which will be addressed in section 4.4.) the inherent reproducibility and stability of a bubble detector should be on the order of a few percent. It seems that the source of these variations may be attributable to the reader being used and the threshold selected for counting. The number of bubbles counted by the first generation readers is critically related to the threshold selected during imaging processing. The threshold determines how intense and large the light spot indicating a bubble must be before it is counted. The intensity and size of the light spot is also strongly dependent on the size of the bubble being imaged.

4.3 TEMPERATURE EFFECTS AND COMPENSATION METHODS

It is known that the response of a bubble detector, because of its composition, i.e., a SHL, is effected by temperature changes. So variations in ambient temperature create the potential problem of detector instability. This instability is exhibited as fluctuations in sensitivity that are proportional to the temperature variations; the greater the temperature variation, the poorer the confidence in the response of the detector. This is clearly not a problem if one is assured that the temperature in the working environment will remain constant or at least within a few degrees of the calibration temperature. But if the detector is to be used when temperature changes are expected or uncontrollable, achieving the highest level of accuracy requires some means of compensation. A plethora of compensation methods have been suggested. A select few are briefly described.

How Temperature Affects Response

Before we can consider the techniques of temperature compensation we must first understand how it is that a BD is affected by temperature. Keep in mind the effect of pressure and temperature on liquid-vapor phase change (Fig. 4.3.1).

Let us begin by stating that an increase in temperature brings about an increase in sensitivity in a two fold manner, by 1) lowering the threshold and 2) increasing the sensitivity above the threshold. This is attributable to the increase in the degree of superheat created by the increase in temperature. The more superheated the liquid, the smaller the r_c . Therefore, neutrons previously incapable of producing a thermodynamically unstable seed bubble (those just below the threshold energy) could now contribute to bubble formation. An equivalent fluence of neutrons above the initial "inhibition energy" or threshold, will produce a greater number of bubbles than they would have produced at a lower temperature. This phenomenon, if ignored, will transform the original detector into a variable "Jekyll and Hyde". This new beast possesses an $R(E)$ which differs from the original creature. This alteration of the $R(E)$ will also mean that the temperature effect is energy dependent. In other words, the increase in response as a function of

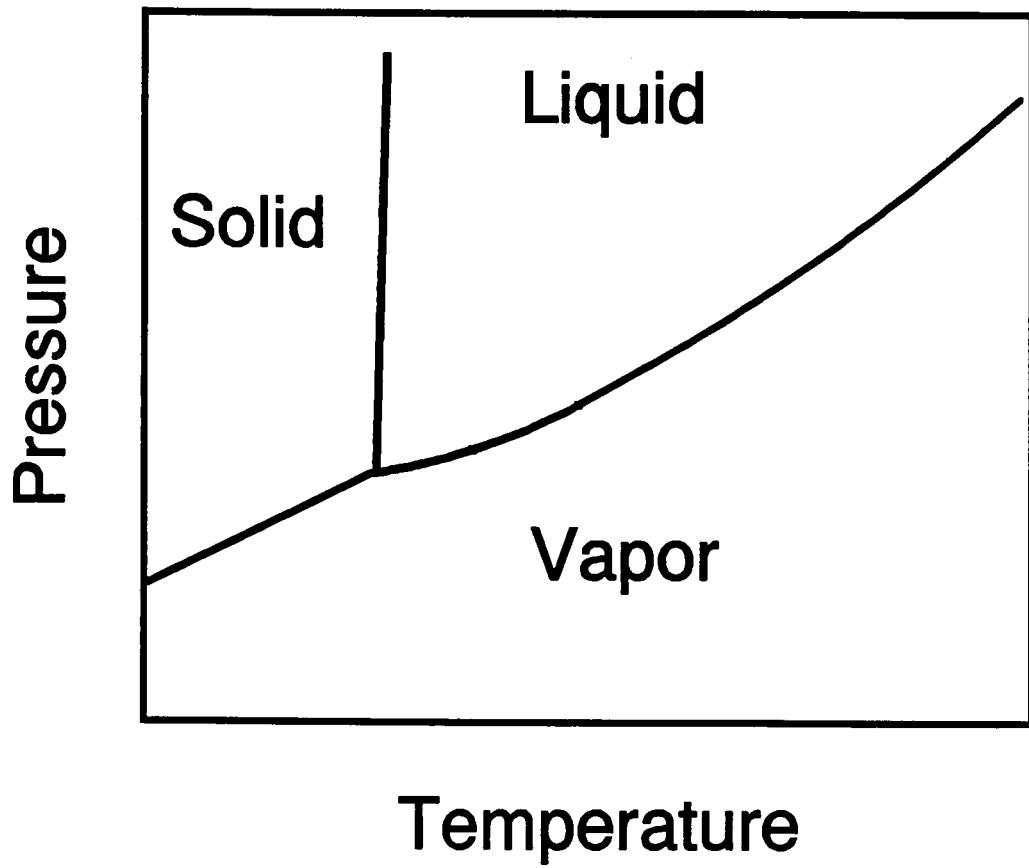


Fig. 4.3.1 Phase diagram in the T,P plane.

temperature will vary from spectrum to spectrum.

An analogy may better illustrate the sensitivity changes brought about by a change in temperature. Consider the home run hitting abilities of a baseball team when playing at home (a function of the average distance the player can hit the ball and the distance to the fence). If we assume the pitcher to be a constant in this analogy, then the frequency of home runs for the team when playing away would be expected to increase when playing an opponent whose home field was smaller, i.e. a shorter distance to the fence. Those players who would just miss hitting it out at home would be more likely to hit one out on the smaller field, while the number of home runs hit by those players normally hitting it out at home would increase only slightly. This makes sense for bubble detectors if we consider the normal home run hitters in our analogy to be representative of the neutrons above the threshold; those with a high probability of producing a bubble at the calibration temperature, the occasional home run hitters as neutrons just below the threshold, while still capable of occasionally causing a bubble to form the probability of doing so is much lower; and the distance to the fence as the r_c . Increasing the temperature has the same effect on bubble formation as does playing on a field with a shorter distance to the fence; the r_c becomes smaller. Those neutrons only occasionally causing a bubble to form at the calibration temperature (or at home) do so more often (with a much higher probability) at a higher temperature (on a shorter field). A decrease in sensitivity would be expected if the temperature were decreased; analogous to playing on a field with a greater distance to the fence.

Pressure Compensation

Presently BTI is employing a means of compensation that attempts to compensate for both of the known culprits responsible for temperature induced response variation. Maintaining a state of equilibrium between the internal vapor pressure of the SHL droplet and the external pressure, a combination of the PAG and atmospheric pressure, is the key to their compensation model. A reservoir of material that expands and contracts with changes in temperature is attached to the

detector, and by utilization of an appropriate mechanical advantage, the pressure within the detector remains virtually constant as the temperature changes. The external pressure applied to the detector is proportional to the combined changes of increased vapor pressure and reduced surface tension experienced by the superheated droplet (Ing 1991). This method of pressure compensation is intended to maintain the SHL at a constant state of superheat, effectively "freezing" the R(E) regardless of the ambient temperature.

Environmental Control

Another approach is to control the temperature environment in which the bubble detector is operated. This could be achieved via a small heat pump type device. The device would provide an adequate amount cooling or heating required to maintain the device at a preset temperature. Currently BTI is working on a small box type device, containing a "heat-disk", to maintain the temperature near normal body temperature (Roy 1991).

Computational Compensation

An alternative to mechanical compensation or environmental control would be to maintain a parallel record of the cumulative response and temperature. This would allow correction of the results by application of derived temperature correction factors. This assumes either short intervals of time between readouts and cognizance of the temperature during bubble formation or a historical record correlating bubble formation and temperature. The frequent reading cycle is impractical for most applications, but a parallel real time detection and temperature logging technique is currently under development at DOSAR.

The first step in the procedure will be to determine the R(E) at a specified calibration temperature, i.e., 25°C. The best possible method of determining the correlation of temperature and energy would be to maintain one variable constant while varying the other. A new investigation is being proposed to assess the temperature effect on response by performing a series of monoenergetic irradiations

while precisely controlling the temperature of the detectors. In this manner the effect of temperature on the $R(E)$ will be determined, i.e., the change in sensitivity at a specific energy as a function of temperature, $\Delta R(E)dT$. This work promises to make significant inroads toward a better understanding of BD response characteristics. Next, the $R(E)$ of each component is segmented into a number of defined EIs with the sensitivity for each EI ($R(EI)$), taken to be the average sensitivity, in $\text{bu}\cdot\text{cm}^2$, in that region. The effective change in sensitivity per $^{\circ}\text{C}$ for each interval will be assessed from the data. Translated, instead of applying a single temperature correction for the change in sensitivity over the entire $R(E)$, (the equivalent of assuming the shape of the $R(E)$ is constant and only the amplitude or sensitivity changes, which we have seen is an incorrect assumption), we will correct for the temperature effects by reestablishing the shape of the $R(E)$ to reflect what the $R(E)$ would be at the irradiation temperature. Because the total response of a BD is a function of the $R(E)$ and the spectrum, and changes in temperature bring about changes in the $R(E)$, to correctly compensate for the temperature induced changes in $R(E)$ a temperature correction factor will be necessary for each spectrum. Temperature corrections derived for one source will not necessarily be applicable to a different source unless the spectra are similar.

Heat induced alteration

One other approach may provide a viable option. Because an increase in temperature effectively increases the superheat of a BD, shifting the $R(E)$ threshold downward in energy and because we desire a detector whose $R(E)$ approximates h_{ϕ} , heating a BD with a higher threshold could shift the threshold down to create a detector with a near dose equivalent response. For example, maintaining a BDS-2500 at a temperature predetermined to achieve the desired threshold shift would eliminate any variation in response associated with temperature fluctuations below the set-point temperature.

4.4 BUBBLE FORMATION, GROWTH AND MEMORY

A normal bubble "life cycle" is characterized by the progression: droplet→formation→growth→recompression→droplet. Fig. 4.4.1. depicts this life cycle. Cognizance of this progression may afford insight to our understanding of such phenomena as changes in sensitivity, bubble growth, bubble memory (the apparent reformation of the same bubble time and time again) and incompressible bubbles. A narrative of this progression is presented, and some inferences and explanations for the observed phenomena are provided.

Bubble Formation

An in-depth description of the currently accepted theory explaining the metamorphosis from incident neutron to bubble is available in the literature (Apfel et al. 1987; Lo 1987). The most recent is offered in the Ph.D. dissertation of Dr. Mark Harper of the U. S. Naval Academy (Harper 1991). In Apfel's model, I assume, the surface tension of the holding medium is assumed to be equivalent to that of the SHL i.e., similar to Glaser's bubble chamber where the entire volume is the SHL (the reason tracks are produced instead of a single bubble in the bubble chamber). Though this may be the case in the SDD, it is certainly not valid during all the stages of bubble formation for the BTI detector. P_0 for the BTI detector is the summation of the atmospheric pressure transferred through the medium, the surface tension of the non-compressible liquid and the force exerted on it by the PAG or "firm...polymer"(Ing and Birnboim 1984). It is my belief that the PAG component of P_0 (P_{PAG}) plays a greater or lesser role in the total P_0 depending upon the present stage expansion or recompression phases. This change is effected by the elasticity and tensile properties of the PAG as it expands and contracts. Because the radius of the seed bubble is much smaller than the SHL droplet during the formation phase, the P_{PAG} is negligible and the surface tension of the SHL is the dominate factor. The P_{PAG} becomes significant once the droplet is consumed and the bubble begins to grow and stretch the PAG.

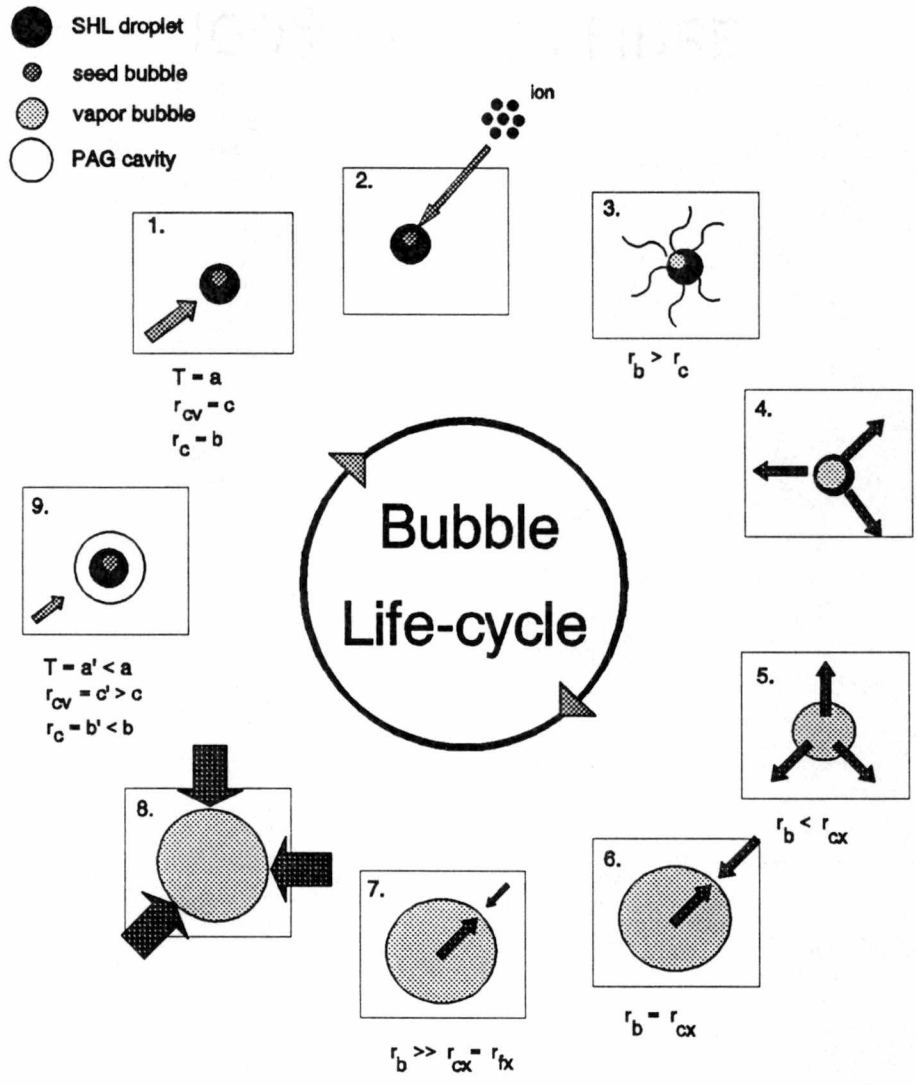


Fig. 4.4.1. The life-cycle of a bubble.

Bubble Growth

At the risk of oversimplification, we will quickly describe the stages depicted in Fig. 4.4.1., and then offer an explanation of these by way of analogy. Frame 1 describes the condition of a virgin SHL droplet, where P_{PAG} is determined by the PAG tension, $T = a$, and the PAG cavity, i.e., the void in the PAG which the droplet occupies (a result of polymerization) with a radius, $r_{cv} = c$. At this point r_{cv} is equal to the droplet radius, r_d . When ions created by an impinging neutron deposit energy within a potential seed bubble, that bubble will begin to grow. Many interactions may occur which produce a seed bubble that does not expand beyond r_c . These bubbles collapse or recondense (frame 2). But once a seed bubble expands to r_c it will violently boil consuming the entire droplet (frame 3). The bubble will continue to grow (frames 4 and 5) until an equilibrium pressure is reached between the internal vapor pressure and the external pressure now primarily from atmospheric pressure P_a and P_{PAG} . The bubble will continue to grow as the PAG stretches (frame 6). Growth of the bubble beyond a certain point will result in damage and consequent loss of tension in the PAG. The radius at which this begins to occur is defined as the critical expansion radius r_{cx} . At some point the bubble is recompressed by application of external pressure, typically hydrostatic (frame 8). After the recompression pressure is released, though the bubble is recondensed, the r_{cv} and r_c have been altered due to a loss of tension in the PAG caused by excessive expansion of the bubble. A bubble that is allowed to expand beyond a r_{cx} will eventually exceed a radius defined as the critical formation radius, r_{fx} (frame 7). This bubble, although recompressed, will no longer remain recompressed once the applied pressure is removed. Let us now attempt to explain what is happening by way of analogy.

The loss of tension in the PAG may be compared to what occurs when inflating a balloon. For the sake of comparison we will subdivide the inflation of the balloon into three stages. The primary stage is characterized by a small radius and slow expansion. At this stage a significant amount of pressure is required to inflate the balloon (frames 3 and 4). The secondary stage is characterized by a sudden expansion of the balloon, a constantly increasing radius and a noticeable decrease in

the pressure required to continue inflating (frames 5 & 6). The tertiary stage, is characterized by a large radius and slow expansion rate (frame 7). This is the point where you blow and blow and the balloon barely enlarges. This last stage is also the point just before the balloon ruptures. Deflating the balloon is analogous to recompression. The transition from the primary to the secondary stage is marked by a sudden increase in the expansion of the balloon and a marked decrease in the pressure required to maintain growth. Because the PAG is elastic, once an initial pressure equilibrium is established, any growth beyond this r_b will constitute a loss in the elasticity the PAG. It is at this point that the r_b has exceed r_{cr} . The transition is made from the secondary to the tertiary stage, marked by a large radius, slow expansion and significant loss in elasticity is the point at which the r_{lx} is exceeded.

Bubble Memory

Bubble memory is manifested as the reappearance or reformation of the same bubble or bubbles nearly every irradiation. At first glance such reappearance would seem particularly odd when one considers that among the thousands of droplets in a single detector, each possessing an equally likely probability for formation, and that these same bubble continue to reform with nearly 100% probability. Let us return to the balloon analogy in order to offer an explanation for bubble memory.

Consider inflating and deflating a single large balloon. Observe the tension of the balloon after it is deflated each time and notice that this tension is directly proportional to the pressure required to inflate the balloon each subsequent time. If the balloon is inflated only slightly for a repetitive number of times, the amount of pressure required to inflate it each successive time is nearly equal and is only slightly less, if less at all. Therefore we may conclude that the tension loss associated with expansion to this radius is practically inconsequential. This is analogous to a bubble which obtains initial pressure equilibrium. However, the larger the balloon is inflated, the easier it is to inflate the next time, and we deduce the greater the radius the greater the tension loss. There exists a radius which, if exceeded, results in a substantial tension loss experienced by the balloon. This radius is defined as the

critical expansion radius, r_{cx} .

Now turning to the formation of bubbles, prior to formation the liquid droplet i.e., the condensed vapor bubble, would possess a finite radius, r_d , and the PAG immediately bounding the droplet can be conceived of as a cavity with radius r_{cv} which, prior to formation, is equal to r_d . After the bubble expands beyond r_{cx} it can be recompressed and condensed to a droplet with radius r_d , but the PAG in exceeding the r_{cx} has lost a substantial fraction of its tension and therefore, when the pressure used to recompress the detector is released, the PAG cavity will no longer maintain its original radius. Consequentially, the new radius of the PAG cavity will be greater than the original r_{cv} . This increase in the cavity radius is proportional to the tension loss due to expansion beyond r_{cx} .

Because the r_{cv} is increased, i.e., the volume of the cavity containing the droplet is larger, part of the droplet passes to the vapor state which increases the vapor pressure in the cavity effectively increasing the degree of superheat of the droplet and decreasing the r_c . Therefore, less energy is required to induce formation. This will mean that the bubble will possess a greater probability of formation and thus form "sooner" in the dose history, i.e., dose as a function of time (which for all practical purposes should be a linear function). A healthy detector should exhibit a linear increase in the number of bubbles formed as the neutron dose equivalent increases. A detector containing bubbles which have exceed r_{cx} will manifest a sudden increase in sensitivity early in the dose history. Fig. 4.4.2. depicts the correlation of bubbles and dose graphically for a normal or healthy bubble detector (one which has been recompressed before any bubbles exceeded r_{cx}) and a detector possessing a number of bubbles that have exceed r_{cx} . This implies that an overresponse will be more significant when measuring lower doses. For a theoretical example consider the responses of two BD-100Rs originally possessing sensitivities of 10 bu per 0.01 mSv and 1 bubble per 0.01 mSv respectively, before and after they develop 3 bubbles exceeding r_{cx} . The results are presented in Table 4.4.1. This suggests that the bubble memory phenomena will have a greater impact on the accuracy when measuring low doses and when encountered in lower sensitivity

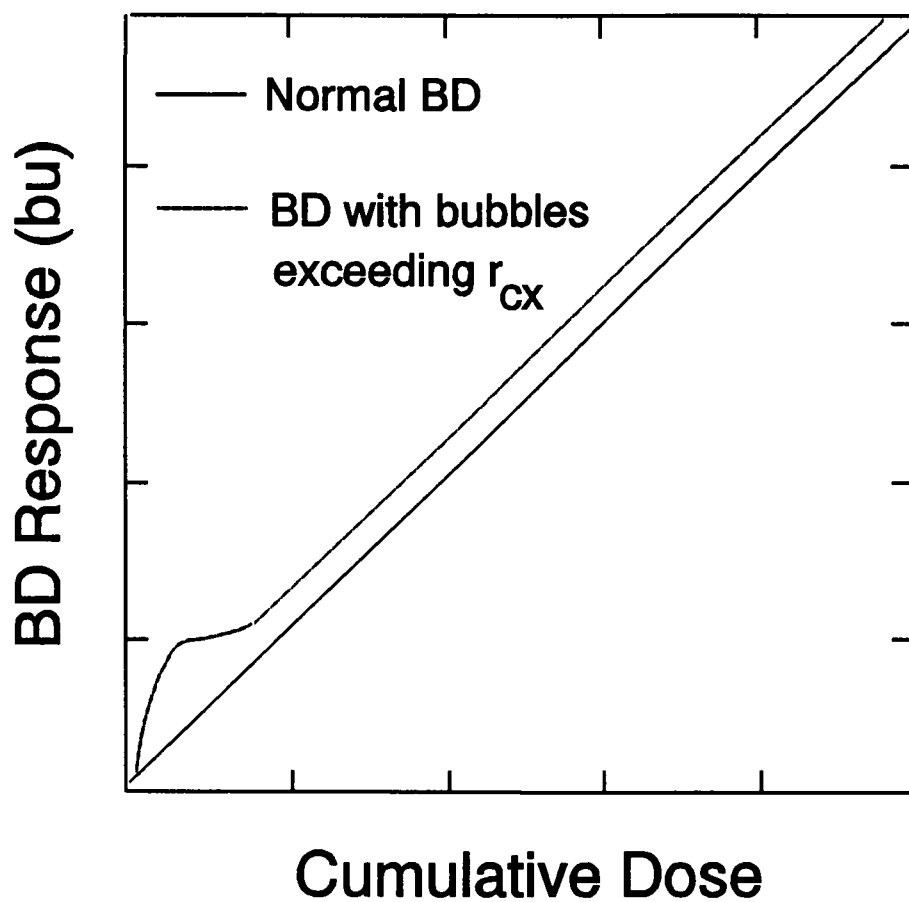


Fig. 4.4.2. Correlative record of BD response and cumulative dose for a normal BD and one which contains bubbles that have exceeded the r_{cx}

Table 4.4.1. Theoretical response of two bubble detectors before and after acquiring three bubbles exceeding r_{cx}

Initial Sensitivity (bu per 0.01 mSv)	Response to 0.01 mSv		Response to 0.1 mSv	
	Before	After	Before	After
1	1	3	10	13
10	10	13	100	103

detectors.

One possible method of reducing the memory problem, other than administratively controlling the size of the bubbles before recompression, would be to nucleate all bubble sites and allow them to grow to the desired size prior to application for measurement purposes. The success of this approach could be empirically verified by repeated irradiations of two sets of detectors, one having all of its droplets nucleated prior to the study and the other comprised of virgin detectors. The nucleation of all the sites for the first set is achievable by placing the detector in a hot water bath. The results from a preliminary study of this theory are currently inconclusive.

Bubble Incompressibility

In order to understand bubbles which appear to be incompressible, let us once again turn to the balloon analogy. Consider the condition of the deflated balloon once it is inflated to the brink of rupture, i.e., exceeding r_{fx} . Once this is done, very little pressure is necessary to inflate it to the same point again. Thus, most of the original tension, which affected the rate of expansion of the bubble, or balloon in our analogy, is expiated. This can be seen by comparing our deflated balloon to either one which has never been inflated or to one which has not been inflated beyond the r_{cx} . The overinflated balloon will be limp in comparison and significantly larger than either of the other two.

The analog to this in the realm of bubble formation would be a bubble which

has expanded to the brink of rupturing the polymer or beyond and is then recompressed. If the r_{cv} after recompression is proportional to the tension loss from excessive expansion as observed in the balloon analogy, it can be inferred that the greater the r_b the greater the degree of superheat of the successive droplet. Once the r_b exceeds $r_{b\infty}$ the successive droplet will find itself in a PAG with a r_{cv} so large that the superheat of the droplet is sufficient to spawn spontaneous formation of the bubble. The net effect of this immediate spontaneous formation will be an "as-if" appearance of an incompressible bubble. Fig. 4.4.3 depicts the tension lost by the PAG as the r_b increases.

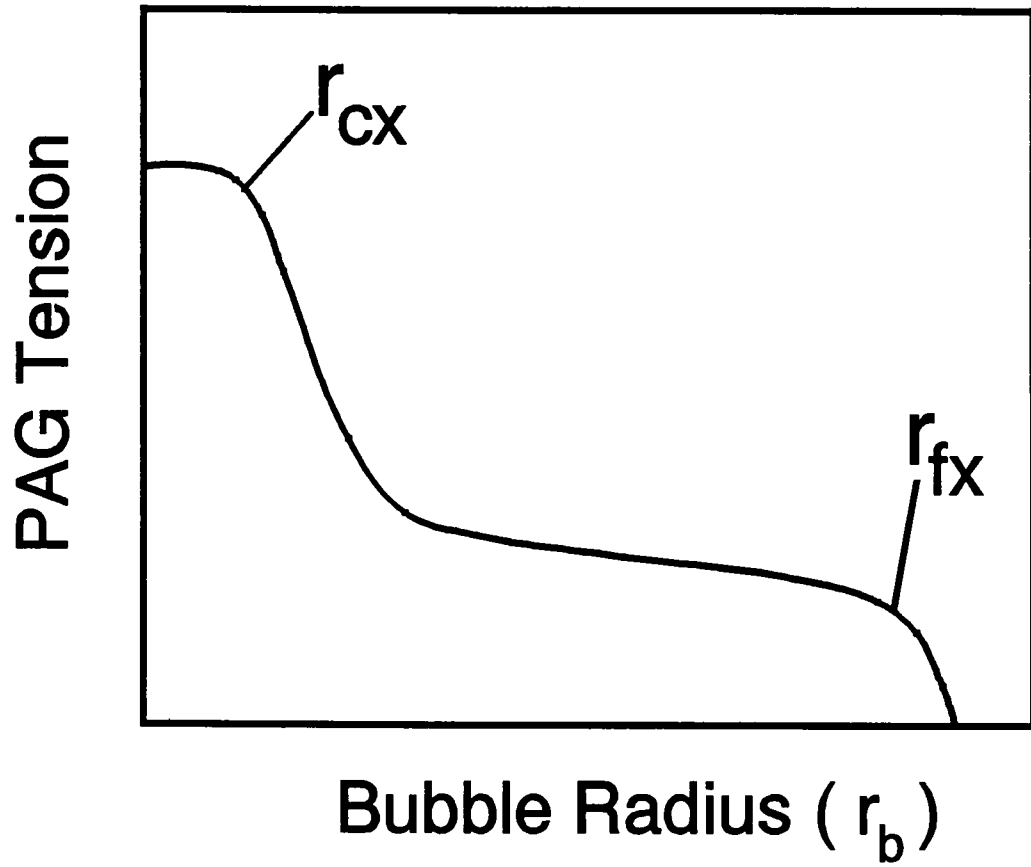


Fig. 4.4.3 PAG tension loss as function of bubble growth.

Chapter V

FUTURE DIRECTIONS AND APPLICATIONS

It is often important to try to see the "big picture", to occasionally stop and evaluate from whence we have come, where we find ourselves presently, and to what lofty heights we expect our dreams to one day take us. With a realistic eye to the past and present, several applications of this technology are discussed, two upon which initial work has begun.

5.1 EXTREMITY DOSIMETRY

An experimental extremity dosimeter was assembled to assess the feasibility of applying bubble detector technology to measure neutron exposure to the extremities. Because the BD-100R possess a "nearly" dose equivalent response it was the material of choice for this experimental model. A sketch of BUDEX (an experimental bubble dosimeter for extremities) appears in Fig. 5.1.1.

A clear plastic disc was affixed to a cross sectional portion of an old bubble detector which was filled with BD-100R material and covered with another plastic disc. The BUDEX was attached to a plastic rod to simulate a finger phantom and irradiated with $^{238}\text{PuBe}$ neutrons. Results indicate that this application holds great promise. BUDEX could provide a good approximation of the neutron dose equivalent delivered to the extremities regardless of neutron spectra or irradiation scenario. This is a feat no TLD based extremity dosimeter could hope of achieving.

5.2 ACCIDENT LEVEL DOSIMETRY/SPECTROMETRY

Based upon a cursory review of the literature available on cavitation theory which attempt to explain the formation of bubbles, in my estimation, a more detailed investigation considering the complex effects of compound surface tension terms, polymer expansion/compression elasticity variables, a reevaluation of the critical

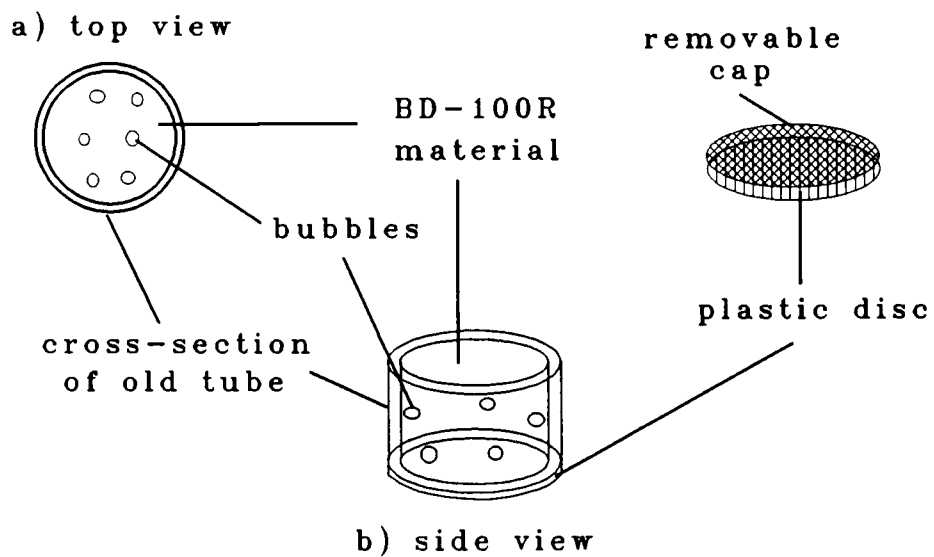


Fig. 5.1.1 Experimental neutron extremity dosimeter (BUDEX).

radius in light of these, and a continuum of energy transfers from elastic scattering is needed. The summation of energy transferred by multiple recoil nuclei which are insufficient to produce a bubble of r_c should be considered. Granted, that for the fluxes typically encountered in standard personnel dosimetry this factor would be negligible; yet, as accident scenario dose rates are approached this factor might be used to our advantage.

Consider a recoil nucleus that deposits an insufficient amount of energy in a SHL droplet to produce a bubble (defined as a subcritical event producing a bubble of subcritical radius, r_s). If we assume an initial temperature of the droplet, t_0 , the energy deposited in producing the subcritical seed bubble as localized heat, according to the "thermal spike" model, would increase the temperature of the droplet within the vicinity of the event to, t_1 . A time interval, t_c , would be required for this heat to dissipate i.e., cool back to the initial t_0 . Assuming that this account of the process is representative of what actually occurs for subcritical events, it is conceivable that a bubble could be formed as the result of a temperature increase produced by the summation of multiple subcritical events. Consequently the effective sensitivity of a detector will be related, in some manner, to the neutron flux impinging on it. The flux at which this phenomenon begins is defined as the critical flux, ϕ_c . If the relationship between ϕ_c and the degree of superheat can be determined, this knowledge might possibly be applied to create an accident neutron spectrometer (ANTS), by maintaining sufficient pressure on a detector (critical pressure p_c) to render it insensitive to neutron flux below ϕ_c . The p_c and ϕ_c will probably vary for each type of detector with greater pressure being required by detectors possessing higher degrees of superheat and larger ϕ_c . Once the ϕ_c is encountered, bubbles would form increasing the pressure in the detector. By employing a pressure relief valve the increase in pressure will be bled off, maintaining the a constant p_c . By using the CPND in this type of application spectral information may be obtainable in the event of a nuclear criticality. The realization of such a device would make more accurate dose and dose equivalent assessment of criticality accidents a reality.

5.3 A "DO-IT-YOURSELF" BUBBLE READER

The challenge that lies before us is developing an inexpensive, yet accurate and reproducible means for counting bubbles. The superior accuracy and reproducibility which the detector itself possesses are often offset by the inherent problem of accurately and reproducibly counting the bubbles. The current generation reader available from BTI is capable of accurately reading approximately 350 bubbles in a single detector. This is under ideal conditions and assumes that μ -droplet detectors are used and that they are read before the bubbles grow large enough to create an overlap problem. This reader can be yours for a mere \$35,000.

The read process is typically: 1) the detector is placed in the reader and an image is displayed on a video monitor, at which time 2) image enhancement may be performed 3) followed by counting. The reader provides the number of bubbles it counted in the image. Because magnification is employed, the upper and lower halves of a detector are imaged and counted separately with the total resulting from the summation of the two counts. It would be nice if the images from which the counts were taken were permanently stored. This would afford an opportunity for manual verification of the numbers and provide a permanent dosimetric record, similar to a glow curve.

Due to budget constraints and the diversity and flexibility required for quality research, I embarked on a quest for a do-it-yourself research grade bubble reader. The following attributes were desired:

- 1) storage of the image for future retrieval and analysis,
- 2) flexibility in image analysis, and
- 3) imaging whole bubbles and not just a bright spot of light reflected through the bubble (characterized by the first generation BTI reader).

By using an off-the-shelf image analysis software package from Jandel Scientific called JAVA, an available video camera, PC-AT and various lighting configurations, this goal was realized. A photo of the reader and an example of an image acquired with it are in Fig. 5.3.1, Fig. 5.3.2. This was achieved for less than \$5,000.


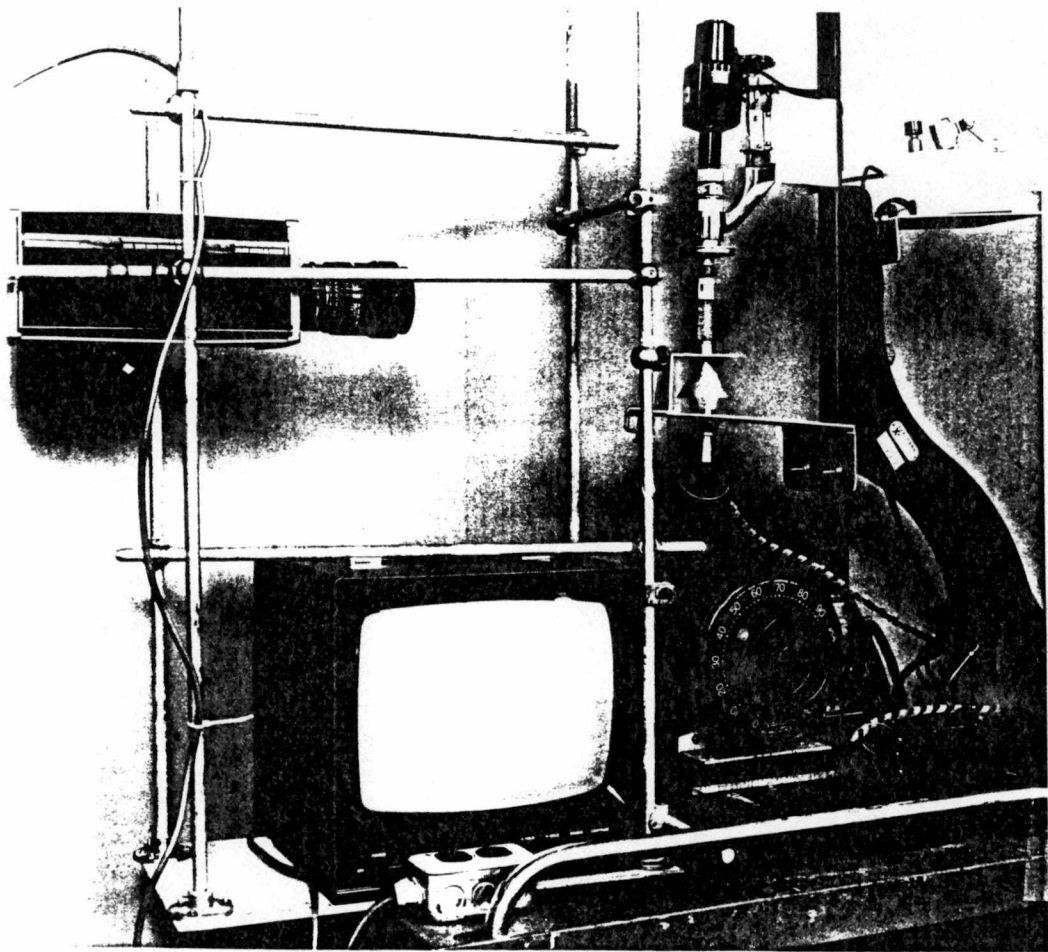


Fig. 5.3.1 A photograph of the do-it-yourself bubble reader.



a)

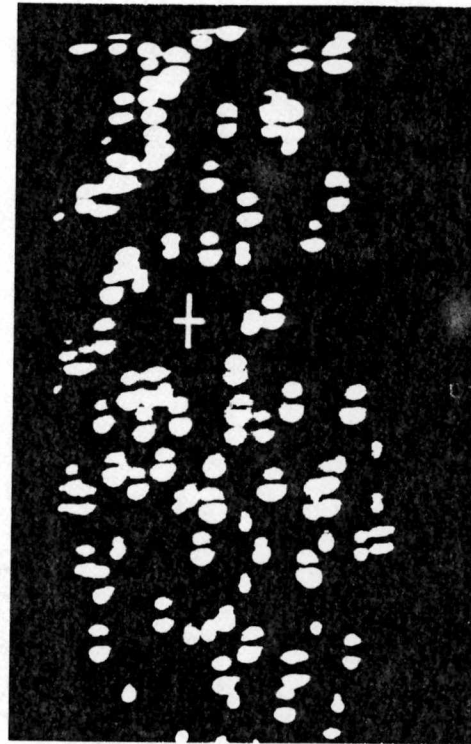

b)

Fig. 5.3.2 An image captured with the D-Y-I reader a) full image, b) magnified image.

This approach to bubble imaging includes several novel aspects: 1) passing light through both ends of the detector which eliminates edge glare caused by reflection of light through the wall of the cylindrical detector and imaging of the "whole" bubble, 2) a counting algorithm that will remove a bubble from the image once it is counted, thus when two or more bubbles overlap, the top bubble after being counted can be removed leaving the partial bubble or bubbles (the curvature of the remaining partial bubble will be completed, counted and removed from the image...etc.) and 3) the introduction of a dye into the PAG to enhance definition of an imaged bubble (the bubble will be clear and the compressed PAG surrounding the bubble will be more dense and thus darker than the rest of the detector PAG).

5.4 DEVELOPMENT OF A COMBINATION AREA NEUTRON SPECTROMETER (CANS)

The information gleaned from improvements to the CPND lead us to believe that superior spectral resolution and, consequently, improved neutron dose equivalent accuracy could be realized through: 1) modification of the TLD component eliminating the need for a phantom, providing greater thermal neutron measuring accuracy and simulating a 4π geometry, 2) inclusion of an additional BD to obtain better spectral resolution in the 0.01 to 1 MeV region and 3) determination of the effect temperature has on the shape of the energy response, $R(E)$, and how to best correct for it. As a result DOE is currently funding the development of the Combination Area Neutron Spectrometer (CANS).

Redesigned TLD

The TLD component of CANS was redesigned to capitalize on the detection of thermal and slow or epi-Cd neutrons without using a phantom. This is possible because the BD components measure the higher energy neutrons. A Harshaw card was used (two Teflon sandwiched TLD-600/700 paired elements in an Al substrate) with one pair sandwiched between Cd filters and the other backed by a Cd filter. The paired TLD-700 is used to subtract the incident photon contribution and the Cd

capture gammas from the TLD-600 response. The Cd sandwiched TLD-600 responds to incident epi-Cd neutrons (> 0.414 eV) and the Cd backed TLD-600 to incident thermal and epi-Cd neutrons. The difference in the two provides an accurate measure of the incident thermal fluence. By placing two of these units back-to-back, a 4π geometry is simulated (Figure 5.4.1).

Additional BDs

The region of greatest change in the fluence-to-dose equivalent conversion factor as defined by ICRP 21 is between about 0.01 MeV and 1 MeV (ICRP 1973). Improving the accuracy of the fluence measurements in this region will spawn a subsequent improvement in the total neutron dose equivalent accuracy. Since the BD-100R and BDS-1500 possess respective thresholds at about 0.1 and 1 MeV, adding a BD with a threshold at about 0.01 MeV (BDS-10) will facilitate measuring neutrons in the regions < 0.01 MeV, from 0.01 - 0.1 MeV, from 0.1 - 1 MeV and from 1 - 15 MeV. Dividing this region into upper and lower regions should improve the overall spectral resolution. BDs possessing thresholds other than these are also being reinvestigated.

Because it utilizes a SHL the BD detector will always inherently possess a degree of temperature dependence. Efforts are currently underway to conduct another set of monoenergetic neutron irradiations at Columbia Universities Radiation Accelerator Research Facility (RARAF) in New York. The experiment will focus on determining how temperature affects a BDs $R(E)$ by irradiating BDs to monoenergetic neutrons at various controlled temperatures, described in Section 4.3. This knowledge, once acquired, will allow us to make inherently more accurate measurements of neutron spectra by altering the BD $R(E)$ equations used in the matrix deconvolution algorithm to reflect what the $R(E)$ s are at the irradiation temperature, instead of applying a gross temperature correction factor to the integrated response which ignores the change in $R(E)$ caused by temperature.

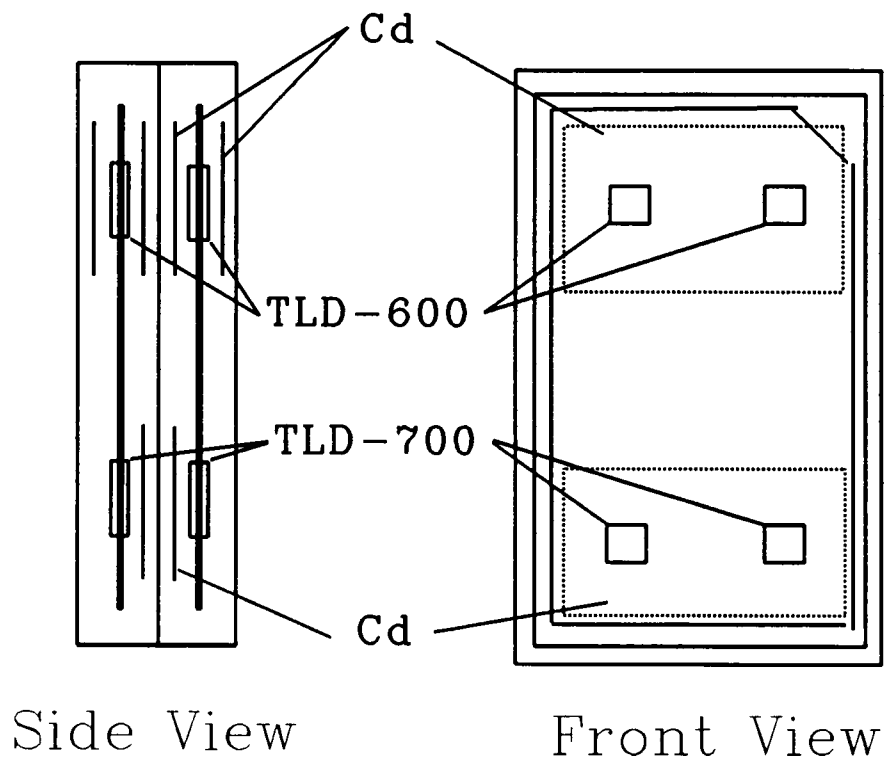


Fig. 5.4.1. Description of the modified TLD component of CANS.

Application to CANS

This newly acquired knowledge will enable us to make more accurate measurements of neutron spectra at temperatures other than those at which the $R(E)$ had been determined by altering the BD $R(E)$ equations used in the matrix deconvolution algorithm to reflect the $R(E)$ at the irradiation temperature. The process will be as follows:

- 1) the temperature at the time of irradiation is recorded,
- 2) a tube correction coefficient, TCC, is applied to the response of each BD to mimic the response of a 1 bu/0.01 mSv calibrated detector
- 3) the $R(EI)$ matrix is modified to reflect the $R(E)$ at the irradiation temperature,
- 4) the matrix is inverted producing equations for the ϕ_{EI} s,
- 5) the TCC values are entered and the equations solved to yield the ϕ_{EI} ,
- 6) application of the averaged h_p for each EI provides the neutron dose equivalent produced in that EI, (H_{EI}), and
- 7) the summation of the H_{EI} s provides the total measured neutron dose equivalent (H_T).

Applying the TCC is analogous to applying an element correction coefficient to individual TLD element readings.

Development is under way with field tests scheduled to include containment of a Texas Utilities BWR, measurements at the TOKAMAK device at Princeton Plasma Physics Laboratory and various pure and mixed field radioisotopic spectra utilizing various shielding configurations at ORNL and NSWC.

5.5 ALTERNATIVE REAL-TIME ACOUSTICAL PROCESSING (ARAP)

Our vision is the development of a real time neutron spectrometer/dosimeter. The realization of this goal will require the synthesis of all we have learned during our BD related research and a cutting edge knowledge of electronics and micro-

processors. The Alternative Real-time Acoustical Processing technique (ARAP), currently under development by the DOSAR Group, may prove to be a step toward realizing this goal. This technique will enable real time application of the BTI's BDs. ARAP will answer the clarion call for a simple device for measuring neutron spectra and calculating dose equivalent. In our mind's eye the devices could resemble those of the artist conceptions in Fig. 5.5.1 and 5.5.2.

It was documented by Apfel that the violent boiling process occasioned by bubble formation transmits a mechanical shock wave manifested as an audible "pop" (Roy et al. 1987). The prototype real time spectrometer, Fig 5.5.1, includes a signal processing board loaded in a laptop computer that will receive and digitize the acoustical signal from a microphone placed inside each detector connected to it. This information will be analyzed and an algorithm will process the information as described in Section 5.4, making appropriate on-line modifications to the R(E)s for temperature compensation as well as on-line calculations of the spectrum, applying the desired average h_{ϕ} to calculate H_{E1} and H_T . Used in this way, ARAP will measure the spectrum and calculate the dose equivalent in real time. These on-line results will be displayed both numerically and as a histogram on the computer screen much as a graphic equalizer. A linear recording of the data will be written to disk.

The device in Fig 5.5.1 will provide a linear correlation of detector response and temperature for the purpose of on-line *a posteriori* compensation for the temperature effects experienced during measurements. An amenity of the system will be its backup features. Three means of verification or reading will be incorporated in the device:

- 1) LCD indication on the detector, of temperature and the cumulative bubble count,
- 2) logging of the cumulative counts and temperature at preset time intervals, and
- 3) should the electronics fail somewhere along the way, the traditional post-event optical counting is still an option.

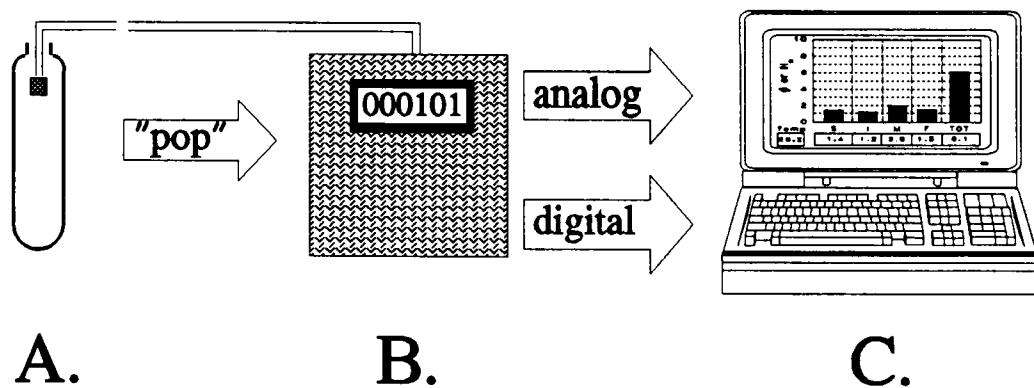


Fig. 5.5.1. Real-time spectrometry: A) "pop" detected by a microphone; B) counted by simple circuitry and displayed; C) multiple detector signals come to a laptop with signal processing board, recorded, processed and spectral results displayed graphically.

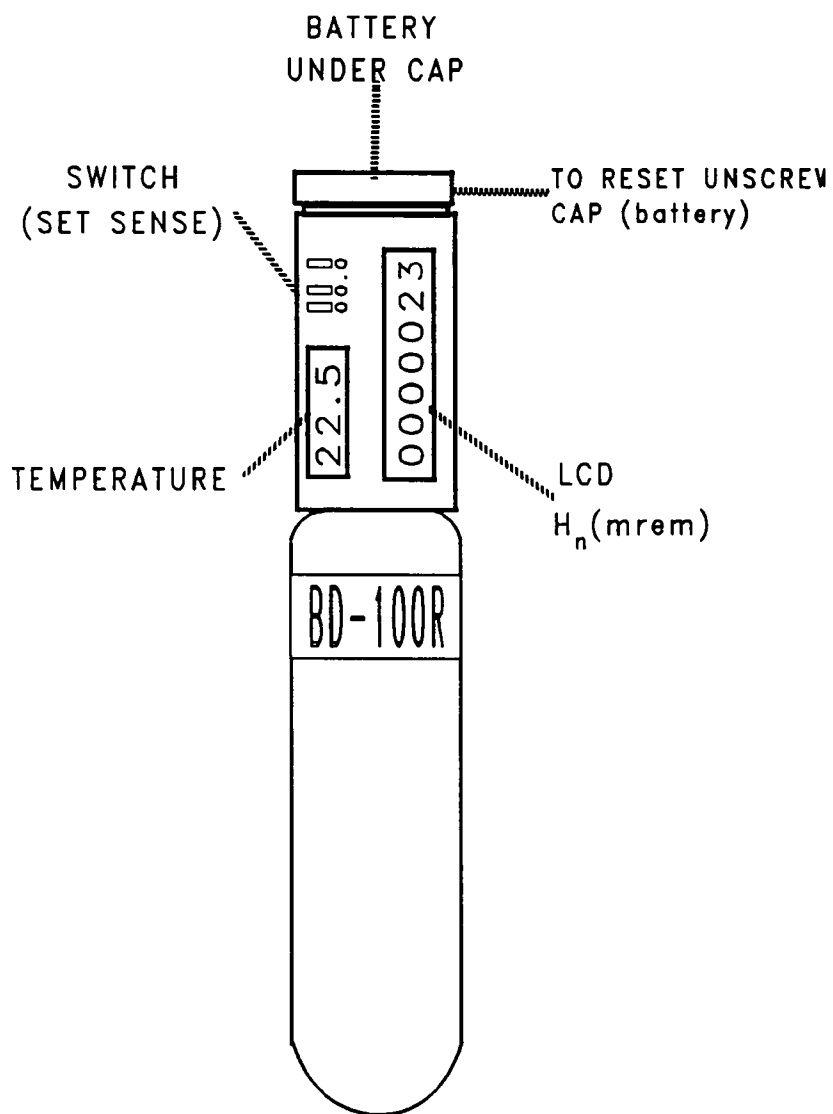


Fig. 5.5.2. Real-time temperature corrected neutron dosimeter using a BD-100R and miniature ARAP.

Chapter VI

SUMMARY AND CONCLUSIONS

The already good performance of the CPND to evaluate the neutron dose equivalent for a variety of neutron spectra both radioisotopic and *in situ* has been improved. The H_T results were within 11% of the reference values (BMS based) for the *in situ* spectra and within 2% of the reference values for the radioisotopic spectra. The low standard deviation and bias suggest improved spectrometric and dose equivalent accuracy and precision ($S = 0.07$ and 0.01 and $B = -0.03$ and 0.01 for the *in situ* and radioisotopic categories respectively). These results were achieved without any *a priori* knowledge of the neutron spectra and with a single algorithm that can be solved using a spreadsheet.

A historical overview of the development of bubble detector technology was presented. A thumbnail sketch of the currently held beliefs on the mechanisms involved in bubble formation and a description of the CPND were provided.

The aspects of the CPND which were modified and the reasoning behind them were discussed. These included:

- 1) refinement of the BD-100R and BDS-1500 response functions,
- 2) reevaluation of the thermal neutron sensitivity of TLD-600,
- 3) redefinition of the energy intervals (EI),
- 4) the a spectrum deconvolution matrix algorithm, and
- 5) the methodology for neutron dose equivalent determination.

The effectiveness of these modifications was assessed by comparing the measured results to both reference values and the original CPND performance. An overall improvement in H_T accuracy over the original CPND of 2% for the *in situ* and 28% for the radioisotopic spectra was observed.

Some explanations were offered regarding:

- 1) useable lifetime,
- 2) observed response variations,
- 3) temperature effects,
- 4) bubble growth,
- 5) bubble memory,
- 6) incompressible bubbles, and
- 7) theory of operation.

Some suggestions were presented for further research and application of this emerging technology. These included:

- 1) extremity dosimetry,
- 2) accident level dosimetry,
- 3) a do-it-yourself bubble reader for research applications,
- 4) development of a Combination Area Neutron Spectrometer (CANS), and
- 5) development of Alternative Real-Time Acoustical Processing (ARAP).

Areas of need

Although the spectral results provided by the CPND and CANS are characterized by a small number of energy intervals or bins (EI), (typically four or five), this should not be viewed as a substantial deficit to its value as an effective and accurate neutron spectrometer/dosimeter. It is believed that this statement is warranted for the following reasons. Considering that there is very little difference in the h_ϕ between thermal energies and 10 keV (according to ICRP 21), a single value of h_ϕ can be applied to the total ϕ in this region. This suggests that only one EI is needed below 0.01 keV, and consequently, that a quantification of the total number of neutrons below 0.01 keV is adequate. Only in specialized situations do radiation environments contain neutrons above 15 MeV (e.g., accelerators and similar devices), therefore, a single EI is all that is needed from 1 - 15 MeV. A single h_ϕ can be then be applied to neutrons in this EI. Also, by dividing the 10 keV to 1 MeV

region into two segments, 10 keV to 100 keV, and 100 keV to 1 MeV, we can improve the spectrometric resolution in this region where the change in h_p is the greatest. This also allows application of a separate h_p to the ϕ in each segment. Thus, we have demonstrated that by strategically defining the EIs one can perform "good" neutron dosimetry with a four interval neutron spectrum. Recall a correction factor derived from 9-to-3 inch ratios (a two point measurement) has historically been applied to albedo dosimeters for energy corrections (Griffith 1979).

What are the areas of greatest need? Are we poised on the brink of a breakthrough in neutron dosimetry? There are still a few ominous problems which must be overcome before bubble detector becomes a "household word" and full blown application of this technology becomes practical in the real world of neutron detection and dosimetry. Some areas of greatest need include:

- 1) storage of the digitized image for a permanent record of the number bubbles in the detector i.e., like a glow curve,
- 2) a reduction in the cost of detectors, which is coming down and will continue as demand increases,
- 3) accumulation of performance data to reinforce acceptance of this new technology by the rank and file in the dosimetry community (this will come with use),
- 4) broadened application i.e., for extremities and photons,
- 5) a low cost reader (the latest generation available from BTI goes for about \$35,000),
- 6) advancement towards overcoming the temperature dependence barrier and its affects on $R(E)$ (advances are being made in this area),
- 7) reduction in size and the geometry of the container to be more conducive to reading and to accommodate the use of multiple detectors in a compact holder and
- 8) a definitive model explaining bubble formation.

Closing remarks

The goal of every dosimetrist should be to provide the most accurate dosimetry possible, utilizing every means within his or her ability to do so. With the probable increase of the neutron quality factor and the push within the U. S. Department of Energy to reduce the current annual dose equivalent limit for radiation workers from 50 mSv to 20 mSv, the ability to provide accurate neutron dosimetry at levels which are typically encountered in the workplace (i.e., 0.1 - 0.5 mSv per quarter) becomes increasingly critical. The history of past Personnel Dosimetry Intercomparison Studies (PDIS) conducted by the DOSAR group at ORNL, indicates that, of the dosimetry systems currently employed, scarce will be those adept enough to weather the impending storm (Sims and Dickson 1985). Although BD technology does not yet offer the perfect dose equivalent device, what technology does? With the anticipated improvements aimed at remedying its weaknesses this technology could threaten to surpass anything currently available, or that is foreseeable in the near future for quick relatively simple and inexpensive, neutron spectral and dosimetric measurements, accurately measuring the neutron dose equivalent received from both known and unknown neutron spectra encountered in the workplace without the necessity of an *a priori* knowledge of the spectra. Utilizing bubble detector technology, one can improve the quality of neutron dosimetry. If development and application continue at their present pace, bubble detector technology may become for the applied health physicist/dosimetrist what the microwave has become for the bachelor, a quick and simple means to achieving a practical end.

REFERENCES

REFERENCES

- Alsmiller R. G., and Barish, J. *The calculated response of ^6LiF albedo dosimeters to neutrons with energies ≤ 400 MeV*, Health Phys., 26:13-28, 1974.
- Apfel, R. E. *The superheated drop detector*, Nucl. Instr. and Meth., 162:603-608, 1979.
- Apfel, R. E., Roy, S. C. *Investigation on the applicability of superheated drop detectors in neutron dosimetry*, Nucl. Instr. and Meth. in Phys. Res., 219:582-587, 1984.
- Apfel, R. E. *Neutron-induced vaporization of superheated liquids: theory and experiment*, Mat. Res Soc. Symp. Proc., 57:57-66, 1987.
- Apfel, R. E., Roy, S. C. and Lo, Y. C. *Prediction of the minimum neutron energy required to nucleate vapor bubbles in superheated liquids*, Phys. Rev., A31:3194-3198, 1987.
- Anderson, M. E. *MLM 1422/TID 4500/UC*, 34, Physics, 1967.
- Block, S., Bryan, J., Prevo, C. and Montan, D. *Laboratory sources enhanced in 0.5 eV to 200 keV neutrons for instrument evaluation*, Health Phys., 13:1025-1031, 1967.
- Buckner, M. A., Casson, W. H., Liu, J. C. *Optimization of the New Combination Personnel Neutron Dosimeter*, Health Phys., 58(Supplement 1), S64, 1990.
- DeMar G. *Censoring America's Christian History*, Biblical Worldview, 6, July 1990.
- DOE Laboratory Accreditation Program for Personnel Dosimetry Systems, *Department of Energy Standard for The Performance Testing of Personnel Dosimetry Systems*, U. S. Department of Energy, Assistant Secretary for Environmental, Safety, and Health. Washington, D. C. 20545, DOE/EH-0027, 1986.
- Eisenhauer, C. M., Hunt, J. B. and Schwartz, R. B. *Calibration techniques for neutron personnel dosimetry*, Radiat. Prot. Dosim., 10:43-57, 1985.
- Eisenhauer, C. M., *Evaluation of dose equivalent per unit fluence for a D_2O -moderated ^{252}Cf neutron source*, Radiat. Prot. Dosim., 9:63-64, 1984.

- Glaser, D. A. *Some Effects of Ionizing Radiation on the Formation of Bubbles in Liquids*, Phys. Rev., 87:665, 1952.
- Griffith, R. V., Hankins, D. E., Gammage, R. B., Tommasino, L., and Wheeler, R. V. *Recent developments in personnel neutron dosimeters-A review*, Health Phys., 36:235-260, 1979.
- Harper, M. J. *A theoretical model of superheated liquid droplet neutron detector*, Ph.D. Dissertation, University of Maryland, 1991.
- Hurst, G. S., Harter, J. A., Hensley, P. N., Mills, W. A., Slater, M. and Reinhardt, P. W. *Techniques of Measuring Neutron Spectra with Threshold Detectors-Tissue Dose Determination*, Review of Scientific Instr., 27:153-156, 1956.
- Ing, H. and Birnboim, H. C. *A bubble-damage polymer detector for neutrons*, Nucl. Tracks and Radiat. Meas., 8:285-288, 1984.
- Ing H., Personal Communication, President, Bubble Technology Industries, Chalk River, Ontario, Canada K0J 1J0, Mar. 11, 1991.
- International Atomic Energy Agency, *Neutron monitoring for radiological protection*, Vienna:IAEA, IAEA Technical Report Series No. 252, 1985.
- International Commission on Radiological Protection. *Data for Protection Against Ionizing Radiation for External Sources*, (Oxford: Pergamon Press) ICRP Publication 21, 1973.
- International Organization for Standardization, *Neutron reference radiations for calibrating neutron measuring devices used for radiation protection purposes and for determining their response as a function of neutron energy*, Geneva: ISO, Draft International Standard ISO/DIS 8529, 1986.
- Ipe, N. E., Busick, D. D. and Pollock, R. W. *Factors Affecting the Response of the Bubble Detector BD-100 and a Comparison of its Response to CR-39*, Radiat. Prot. Dosim., 23:135-138, 1988.
- Ipe, N. E. and Busick, D. D. *BD-100: The Chalk River Nuclear Laboratories' Neutron Bubble Detector*, Stanford University, SLAC-PUB-4398 Stanford, California, USA, 1987.

- Knoll, G. F. *Radiation Detection and Measurement*, John Wiley and Sons, Inc., 1979.
- Kuyper, A. Principles of Sacred Theology, Baker Book House Co., Grand Rapids, Michigan, p. 78, 1980, (Encyclopedia of Sacred Theology ... Its Principles, Charles Scribner's Sons, 1898).
- Liu, J. C. *The Development, Characterization, and Performance Evaluation of a New Combination Type Personnel Neutron Dosimeter*, Ph.D. Dissertation, Texas A&M University, College Station, Texas, 1989 [Also Oak Ridge National Laboratory, Oak Ridge, Tennessee 37831, ORNL-6593, 1989].
- Liu, J. C. and Sims, C. S. *Characterization of the Harsh Albedo Tld and the Bubble Detectors BD-100R and BDS-1500*, Radiat. Prot. Dosim., 32:21-32, 1990.
- Liu, J. C. and Sims, C. S. *Performance Evaluation of a New Combination Personnel Neutron Dosimeter*. Radiat. Prot. Dosim. 32:33-43, 1990.
- Lo Y. C. *Characterization of a neutron detector based on superheated drops*, Technical report 87-1, Yale University, 1987.
- Lorch, A. E. *International Journal of Applied Radiations and Isotopes*, 26:585-591, 1973.
- Massand, O. P. and Venkataraman, G. *The Neutron Spectrum of Plutonium Fluoride*, Nucl. Instr. and Meth., 121:405-506, 1974.
- Pollock R. W., *Current Developments with Bubble Detectors*. Siemens Gammasonics, Inc., Des Plaines, Illinois, USA (Technical Note), 1989.
- Roy D., Personal Communication, Technology Applications Manager, Bubble Technology Industries, Chalk River, Ontario, Canada K0J 1J0, Jan. 9, 1991.
- Roy, S. C., Apfel, R. E. and Lo, Y. C. *Superheated Drop Detector: A Potential Tool in Neutron Research*, Nucl. Instr. and Meth., A255:199-206, 1987.
- Schwartz, R. B. and Hunt, J. B. *Measurement of the Energy Response of the Superheated Drop Neutron Detectors*, Radiat. Prot. Dosim., 34:377-380, 1990.
- Seitz, F. *On the Theory of the Bubble Chamber*, Phys. Fluids, 1:2-13, 1958.
- Sims C. S. and Dickson H. W. *Neutron dosimetry intercomparison studies*, Radiat. Prot. Dosim., 10:331-340, 1985.

Swaja, R. E. and Sims, C. S. *Neutron Personnel Dosimetry Intercomparison Studies at the Oak Ridge National Laboratory: A Summary (1981-1986)*, Health Phys. 55:549-564, 1988.

Van Til, C. Common Grace and The Gospel, Presbyterian and Reformed Publishing Co., Phillipsburg, New Jersey, pp. 5, 63, 1972.

Vylet, V., Swaja, R. E., Prêtre, S., Valley, J. F. and Lerch, P. *On the use of the '9-to-3' ratio with albedo and fission track neutron personnel doseimeters*, Radiat. Prot. Dosim., 27:29-33, 1989.

Werle, H. *Kernforschungszentrum Karlsruhe*, 4/70-25, 85, 1970.

APPENDIX

THE SPECTRAL NEXUS: UNDERSTANDING THE RELATIONSHIP BETWEEN RESPONSE FUNCTIONS AND NEUTRON SPECTRA

The common practice of primarily employing the average energy as the identifying feature of a neutron spectrum is, though unintentional, often misleading. Because the response curve of most dosimeters is drastically different from that of the h_{ϕ} , it becomes very difficult for current dosimeters to measure the neutron dose equivalent of an unknown or mixed neutron field. One of the underlying difficulties stems from the rapid decrease in h_{ϕ} from 1 to 0.01 MeV. As the incident neutron energy decreases from 1 to 0.01 MeV, an increasingly larger number of neutrons is required to produce the same biological effect. The difference in h_{ϕ} in this region is as great as a factor of 33, from 9.9 pSv-cm² at .01 MeV to 327 pSv-cm² at 1 MeV. Consequently, the same dose equivalent produced by 33 0.01 MeV neutrons would require only a single 1 MeV neutron.

Dosimetrists rarely deal with mono-energetic neutron exposures. More typically the neutron fields encountered are unknown and polyenergetic. The exigency of this situation dictates that careful consideration of the entire spectrum is necessary. Unfortunately, and to the demise of many investigators, this importance is frequently minimized. Such minimization is often done for the sake of simplification. But, this oversimplification can spawn unwarranted inferences, contribute to the development of erroneous or false models and inhibit the formulation of valid explanations for observed phenomena. Case in point.

Ipe et al. conducted a series of experiments for the purpose of assessing the energy dependence of the BD-100 (Ipe et al. 1988). The BD-100 and BD-100R are synonymous, therefore, BD-100R will be used for the remainder of this work (Pollock 1989). The average energies (given in MeV) of the sources used in the Ipe et al experiments are, 4.5 for ²³⁹PuBe, 2.3 for PuB, 2.15 for ²⁵²Cf, 0.9 for PuF, and 0.5 for

PuLi. The data acquired by Ipe et al appears to indicate that an increase in the BD-100R sensitivity is to be expected as the incident neutron energy decreases. Since the average energies fall well within the flat region of the BD-100R response curve (i.e. the region above 150 keV, see Fig. 2.2.1 in the body), would it not seem reasonable, upon cursory examination, to expect the BD-100R response to be more or less identical for each of these sources? There must be a logical explanation for the increase in sensitivity observed by Ipe et al. Obtaining such cognizance requires a more in-depth look into what is actually occurring.

Let us consider the interrelationships of the BD-100R $R(E)$, h_\bullet and the spectral shape as we try to understand the organic nexus existing between these elements and the observed phenomena.

Response curve and h_\bullet

First note that, because the sensitivity of the BD-100R is the same for all neutrons above 150 keV, in this region the BD-100R responds more like a fluence device than it does a dose equivalent device. A simple illustration may help realize this point. Consider a BD-100R that receives 0.5 mSv (50 mrem) from three monoenergetic neutron beams of energies, $E_1 = 5.0$ MeV, $E_2 = 2.76$ MeV, and $E_3 = 513$ keV. Based on an h_\bullet of 408 pSv-cm² for E_1 and E_2 and 203 pSv-cm² for E_3 , the fluences required to induce 0.5 mSv are 1.23×10^6 cm⁻² for E_1 and E_2 and 2.46×10^6 cm⁻² for E_3 . Given a sensitivity of 1 bubble-10 μ Sv⁻¹ (1 bu mrem⁻¹) when calibrated to ²³⁸PuBe, the sensitivity at all three energies is, 4×10^{-5} bu-cm². Therefore, 49 bubbles would be produced by a 0.5 mSv dose equivalent delivered by neutrons of E_1 (5.0 MeV) and E_2 (2.76 MeV) and 99 bubbles by 0.5 mSv of E_3 (513 keV) neutrons. Inferentially, for neutrons above 150 keV the response of the BD-100R reflects the number of neutrons traversing the device rather than the dose equivalent delivered by the neutrons, i.e. fluence indication.

Spectral Nexus

The implication of this phenomena becomes even more complex when attempting to detect an integral dose equivalent delivered by impinging neutrons that are polyenergetic, i.e. a spectrum. When measuring the same dose equivalent delivered from two different spectra, the response of the BD-100R will be more pronounced for the spectrum with the larger fluence above 150 keV, regardless of the spectrum's average energy.

Analysis of the response function of the BD-100R and a plot of the neutron energy spectra for $^{238}\text{PuBe}$ and unmoderated ^{252}Cf (average energies of 4 MeV and 2.15 MeV respectively) will illustrate this distinction more clearly, i.e. Fig. A.1. Inspection of the spectra after normalization to a 0.01 mSv (1 mrem) fluence equivalent reveals that the unmoderated ^{252}Cf spectrum contains a greater number of neutrons in the energy region that corresponds to the flat segment of the BD-100R response curve than does the $^{238}\text{PuBe}$ spectrum; ergo a greater sensitivity to unmoderated ^{252}Cf than $^{238}\text{PuBe}$. Another attribute that will influence the BD-100R's response is the width of the spectrum, i.e. broad verses narrow.

The source spectra used in the Ipe et al study, excluding $^{239}\text{PuBe}$ and unmoderated ^{252}Cf , are characterized by fairly narrow neutron energy distributions. With each decrease in average energy a corresponding increase in the total number of neutrons or fluence is required to produce the same dose equivalent. Therefore, when measuring the same delivered dose equivalent as the average energy decreases, an increase in response would be expected.

Although the average energy of unmoderated ^{252}Cf (2.15 MeV) is only slightly lower than that of PuB (2.3 MeV), the difference in spectrum shape is significant. A larger fraction of the broad fission spectrum lies between 150 keV and 1 MeV than does the more narrow PuB spectrum. It is this greater number of neutrons per unit dose equivalent above 150 keV that contributes the increase in sensitivity for this broad unmoderated ^{252}Cf spectrum, a more stark increase even than would be expected from a more narrow spectrum (like the other sources used by Ipe et al) with identical average energy. The response to a $^{239}\text{PuBe}$ spectrum (4.5 MeV average

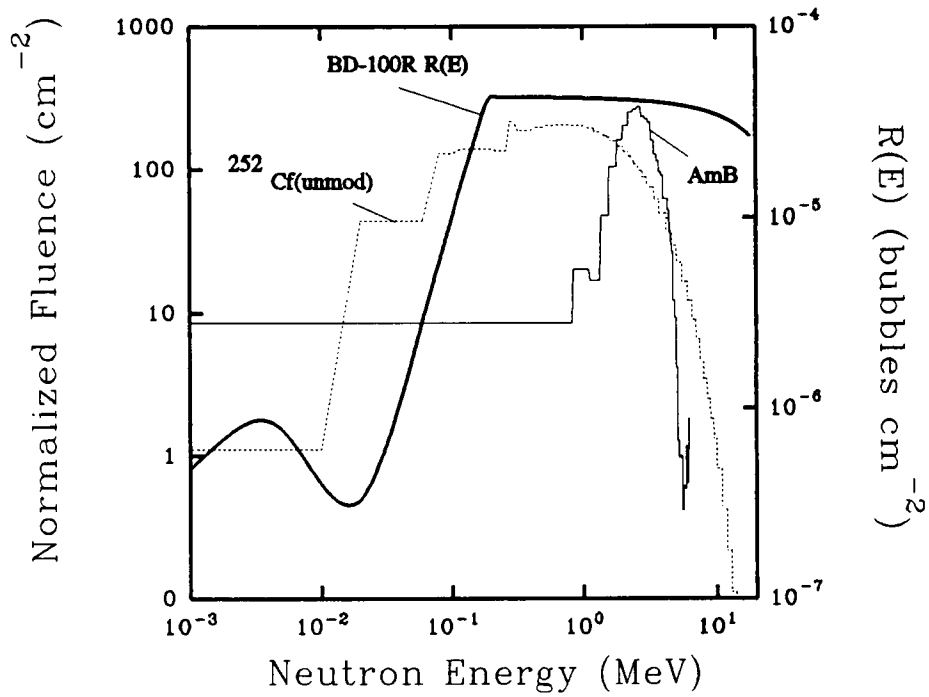


Fig. A.1 The BD-100R $R(E)$ and $^{241}\text{AmBe}$ and $^{252}\text{Cf}(\text{unmod})$ spectra normalized to 0.01 mSv.

energy) would be even less than that to $^{238}\text{PuBe}$, therefore the increase in response to unmoderated ^{252}Cf observed by Ipe et al would appear even more pronounced.

Thus, spectral differences manifest themselves as deviations or variations in the response of the BD-100R when used to measure dose equivalent from a spectrum other than the calibration spectrum, i.e., the response is spectrum dependent. A similar, yet more pronounced effect is experienced by all current neutron dosimetry techniques.

When a Sv is not a Sv?

Because the variations in a detector's response depend on the differences between the measured and calibration spectra, the response of the BD-100R or any other detector may be quantified for any spectra by obtaining reference spectral information and folding it into the response function. This provides both a spectrum specific sensitivity and an answer to the question of how much the response can be expected to vary from one spectrum to another. This has been accomplished for eleven radioisotopic neutron sources obtained from the literature as noted in Table A.1. The sources are: ^{252}Cf unmoderated and moderated by D_2O , (^{252}Cf and $^{252}\text{Cf}[\text{unmod}]$), $^{244}\text{CmBe}$, ^{241}AmB , $^{241}\text{AmBe}$, ^{241}AmF , $^{241}\text{AmLi}$, $^{239}\text{PuBe}$, $^{238}\text{PuBe}$, ^{238}PuC and ^{238}PuF . The derived source sensitivities and dosimetric conversion conventions calculated are the next topic of discussion.

Predicted sensitivities in several radio-isotopic spectra

Various investigators have published spectra for these sources. For the sake of comparison, values were calculated for different spectra of the same radioisotopic neutron source. A graph of the published spectrum was imaged and digitized using a video camera, digitizing board and imaging software. The image was calibrated in both the x and y plane in concurrence with the axis of reference. Then points were selected along the curve representing the spectrum providing an x-y coordinate corresponding to the selected point. This information was exported to a spreadsheet for manipulation. Computations based on ln-ln interpolation were performed to

determine the relative abundance of the neutrons in each spectrum from 0.025 eV to 15 MeV broken down into 20 keV intervals. To normalize the spectra to a single neutron, the value for each 20 keV interval was divided by the total number of neutrons for each reference spectrum (i.e., the sum of all the EIs); ergo, each spectrum represents the relative abundance or the fraction of single source neutron broken down into 20 keV intervals. The ICRP 21 h_p , BD-100R R(E) and TLD-600 R(E) were also entered into the spreadsheet and interpolated over the corresponding 20 keV EIs. The h_p was folded into each spectrum i.e., the h_p of each 20 keV ICRP 21 interval was multiplied by the ϕ of its corresponding spectrum interval. Because the spectrum is representative of the distribution of a single source neutron, the summation of these EI dose equivalents provides the dose equivalent per each neutron emitted from the source. This is commonly known as the spectrum averaged ICRP 21 fluence-to-dose equivalent conversion factor. Dividing each 20 keV interval by this spectrum averaged h_p yields a spectrum that, when the h_p is applied, yields 0.01 mSv, i.e., a 0.01 mSv (1 mrem) normalized spectrum. This procedure was followed for each of the sources under investigation. The response of a detector can then be estimated by folding the detectors R(E) into the 0.01 mSv normalized spectrum. This yields a calculated source specific sensitivity in detector response per 0.01 mSv (mrem). The source specific sensitivities of the TLD-600 and the BD-100R were calculated for each of the available spectra. The results of these calculations are provided in Table A.1. In addition to the source specific sensitivities, the calculated fluence and dose equivalent weighted average energies and spectrum averaged fluence-to-dose equivalent conversion factors are provided.

Source-specific Correction Factors

These calculated sensitivities can then be applied to produce correction factors as follows,

$$C_s = S_r / S_c, \quad (\text{A.1})$$

Table A.1. Calculated values of $\bar{E}(\phi)$, $\bar{E}(H)$, \bar{h}_ϕ and BD-100R response for several radioisotopic neutron sources.

Source ^a	Reference	$\bar{E}(\phi)^c$ (MeV)	$\bar{E}(H)^d$ (MeV)	\bar{h}_ϕ^e (10^{-10} Sv-cm ²)	TLD-600 (mR/mrem)	100R R(E) ^f (bu/mrem)
²³⁸ PuBe	Kozlov	5.1	5.12	4.08	0.38	0.94
²³⁸ PuBe(low) ^b	Kozlov	4.86	4.94	4.01	0.42	0.96
²⁴¹ AmBe	Capgras	4.73	4.82	4.01	0.42	0.97
²³⁹ PuBe	Capgras	4.63	4.73	3.99	0.43	0.97
²⁴¹ AmBe(low) ^b	Capgras	4.56	4.73	3.93	0.46	0.99
²³⁹ PuBe(low) ^b	Capgras	4.5	4.67	3.93	0.46	1.00
²⁴⁴ CmBe	Capgras	4.5	4.65	3.94	0.46	0.99
PuC	Lorch	4.48	4.48	4.09	0.46	0.95
²⁴⁴ CmBe(low) ^b	Lorch	4.25	4.54	3.8	0.38	1.03
AmBe	ISO	4.15	4.52	3.73	0.52	1.03
PuC(low) ^b	Lorch	3.72	3.8	3.97	0.56	1.00
Cf(unmod)	Lorch	2.81	2.86	3.93	0.48	1.03
AmB	Lorch	2.76	2.78	4.00	0.57	1.01
AmB	ISO	2.73	2.79	3.96	0.54	1.02
AmB(low) ^b	Lorch	2.72	2.76	3.96	0.56	1.02
Cf(unmod)(lo	Lorch	2.44	2.61	3.68	0.68	1.1
Cf(unmod)	ISO	2.14	2.47	3.35	0.85	1.2
PuF	Anderson	1.63	1.67	3.64	0.77	1.14
AmF	Lorch	1.61	1.63	3.69	0.75	1.12
AmF(low) ^b	Lorch	1.47	1.54	3.5	0.84	1.18
PuF(low) ^b	Anderson	1.44	1.56	3.36	0.91	1.23
PuF	Massand	1.4	1.47	3.43	0.88	1.21
PuF(low) ^b	Massand	1.4	1.47	3.43	0.88	1.21
Cf(D ₂ O)	ISO	0.546	2.22	0.926	6.38	1.25
AmLi	Werle	0.459	0.625	1.7	2.69	2.06
AmLi(low) ^b	Werle	0.439	0.624	1.66	2.75	2.05

^a The data for all spectra, except those from ISO, were obtained from a digitized image of each spectrum from the referenced literature.

^b The fluence in the low energy range was estimated by extrapolating linearly from the value at the lowest available energy to zero at $E = 0$ MeV according to ISO/DIS 8529 Annex A (ISO/DIS 1986).

^c $\bar{E}(\phi)$ is the fluence weighted average energy.

^d $\bar{E}(H)$ is the dose equivalent weighted average energy defined by ISO/DIS 8529 section 3.19 (ISO/DIS 1986).

^e \bar{h}_ϕ was derived in the manner described by ISO/DIS 8529 section 3.18 using ICRP 21 h_ϕ .

^f The BD-100R response was determined by folding a 0.01 mSv (1 mrem) normalized spectrum of each source into the response function (R(E)) of the BD-100R.

where

S_t = sensitivity to spectrum being measured (bu mSv⁻¹), and

S_c = sensitivity to calibration spectrum (bu mSv⁻¹).

The calibration factors are applied to the reported dose equivalent result H_r ,

$$H_r = bu * S_c, \quad (30)2$$

where

bu = number of bubbles in the detector.

The variation in the sensitivity of the bubble detector to the test and calibration spectra is corrected for by using this equation,

$$H_c = C_s * H_r, \quad (31)3$$

where

H_c = corrected dose equivalent response (mSv),

C_s = correction factor for the spectrum of interest, and

H_r = raw response in mSv to the spectrum of interest.

VITA

The author was born to James and Martha Buckner, of Kingsport, Tennessee, on June 22, 1963. He received a B. A. in Physics and Psychology from Carson-Newman College in 1986. In March of 1987 he was employed by Martin Marietta Energy Systems as a Health Physics technician at Oak Ridge National Laboratory (ORNL). From May of 1988 until September of 1989 he worked in the Centralized External Dosimetry Processing Center, during which time he received an R&D-100 award for his participation in the collaborative development of the Harshaw Model 8800 Thermoluminescent Dosimetry System. Since September of 1989 he has worked as a research associate in the Dosimetry Applications Research Group (DOSAR) at ORNL.

He entered the Nuclear Engineering Department of the University of Tennessee as a part-time graduate student in 1987. He is a member of the Contemporary Christian band Emmaus Road and is serving as a deacon at Covenant Presbyterian Church Oak Ridge, Tennessee. In December of 1991 he was awarded the Master of Science degree in Nuclear Engineering. He plans to pursue, God willing, a PhD., combining the disciplines of Health Physics/Nuclear Engineering, Electrical Engineering and Computer Sciences in design and development of nuclear instrumentation.